



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (5-2011)

Chemical Test Operator Name (Print) <i>Justin Wallerich</i>		
Location <i>Cooperstown - Griggs Co SD</i>	Intoxilyzer® Serial Number <i>80-003071</i>	
Gas Lot Number <i>16512080A2</i>	Gas Cylinder Number <i>30</i>	Gas Expiration Date <i>08-01-2014</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 - A. *0.080* AC
 - B. *0.080* AC
 - C. *0.081* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Breath Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature <i>[Signature]</i>	Date <i>01/11/2013</i>
Reviewed By (Crime Laboratory Use Only) <i>Deb Kashner</i>	Date <i>16 Jan 2013</i>

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003071
Location = COOP 8164.13.00 06/09
01/11/2013 14:09

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:09
02 Std. Gas	0.080	14:10
03 Room Air	0.000	14:10
04 Std. Gas	0.080	14:10
05 Room Air	0.000	14:11
06 Std. Gas	0.081	14:11
07 Room Air	0.000	14:12

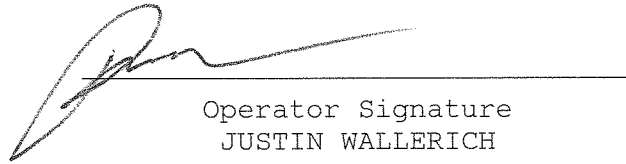
Lot No = 16512080A2

Cyl No = 30

Exp Date = 08/01/2014

County = 20

Oper No. = 011017


Operator Signature
JUSTIN WALLERICH

Remarks:

Form 106-I8000