



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59281 (03-2014)

Serial Number 80-005358	Instrument Location LAMOURE COURTHOUSE LAMOURE SHERIFF'S DEPARTMENT LAMO
Reason for Install/Repair <input type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): n/a
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer® 8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>[Signature]</i> NDA# 276	Date 01/16th 2015
Reviewed By (Crime Laboratory Use Only) <i>Deb Kasher</i>	Date 26 Jan 2015

This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Certified By: *Charles E. Ede* Certified Date: **23 Nov. 2016**

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005358
Location = LAMO 8164.13.00 06/09
01/16/2015 16:21

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=-|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=-|
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 33913080A4
Standard Cyl #? 46
Standard Expiration? 01/01/2016
Oper No? 039706

Flow Cal. Date: 04/17/2014
Slope 622
Intercept -324577

IR Calibration Date: 05/13/2013
 3um 9um

0th Coef(*100): -11171 -20531
1st Coef(*100): 268394 142377
2nd Coef(*100): 3691 1326
H2O adj(mg/l*10k): 575 624

***** Printer Test End *****

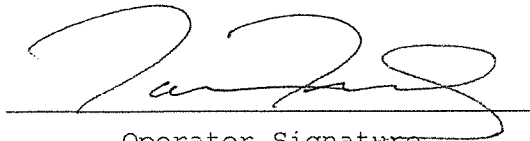

Operator Signature
THOMAS HERZIG

Remarks:


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005358
Location = LAMO 8164.13.00 06/09
01/16/2015 16:27

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:28
02 Std. Gas	0.081	16:28
03 Room Air	0.000	16:29
04 Std. Gas	0.081	16:29
05 Room Air	0.000	16:30
06 Std. Gas	0.082	16:30
07 Room Air	0.000	16:31

Lot No = 33913080A4
Cyl No = 46
Exp Date = 01/01/2016
County = 23 Oper No. = 039706


Operator Signature
THOMAS HERZIG

Remarks:


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005358
Location = LAMO 8164.13.00 06/09
01/16/2015 16:32

Test	AC	Time
01 Room Air	RFI*	16:34
02 Room Air	0.000	16:34

*Invalid Test
Inhibited - RFI

Sub Name = HERZIG, THOMAS JAMES
Sub DOB = 08/22/1972
Sub Sex = Male Weight = 200
Test = DUI Cit = NA
Dr. Lic. = ND/HER733104
Lot No = 33913080A4
Cyl No = 46
Expiration Date = 01/01/2016
County = 23 Oper No. = 039706



Operator Signature
THERZIG HERZIG

Remarks:

Form 106-18000