



ETHANOL BREATH STANDARD CYLINDER REPORT
OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59262 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Hinton Rick</u>		
Location: <u>Class County Jail</u>		
Intoxilyzer @ Serial Number: <u>80-004946</u>		
Lot Number: <u>668180</u>	Cylinder Number: <u>76</u>	Expiration Date: <u>9-21-11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>79</u> %		
Test 2: 0. <u>79</u> %		
Test 3: 0. <u>78</u> %		
(ATTACH TEST RECORD)		

Rick Hinton 3554
Chemical Test Operator Signature

1-17-11
Date

Deb Kashner
Reviewed By

24 Jan 2011
Date

80-004946
P. 67 of 68
KTM

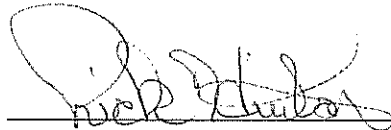
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004946
Location = CASS 8164.13.00 06/09
01/17/2011 09:24

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:25
02 Std. Gas	0.079	09:25
03 Room Air	0.000	09:26
04 Std. Gas	0.079	09:26
05 Room Air	0.000	09:27
06 Std. Gas	0.078	09:27
07 Room Air	0.000	09:27

Lot No = 668180
Cyl No = 76
Exp Date = 09/21/2011
County = 09 Oper No. = 029920

 3554

Operator Signature
RICK HINTON

Remarks:

Form 106-I8000

80-004946
P. 68 of 68
FM