



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: Adam Krabbenhoft		
Location: LaMoure County Courthouse		
Intoxilyzer® Serial Number: 80-004942		
Gas Lot Number: 709352	Gas Cylinder Number: 14	Expiration Date: 12-23-11
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0.080 %		
Test 2: 0.080 %		
Test 3: 0.080 %		
(ATTACH TEST RECORD)		

Adam Krabbenhoft
Chemical Test Operator Signature

2-1-11
Date

Deb Keshner
Reviewed By

15 Feb 2011
Date

80-004942
P. 59 of 60
SM


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004942
Location = LAMO 8164.13.00 06/09
02/01/2011 08:47

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:49
02 Std. Gas	0.080	08:49
03 Room Air	0.000	08:49
04 Std. Gas	0.080	08:50
05 Room Air	0.000	08:50
06 Std. Gas	0.080	08:51
07 Room Air	0.000	08:51

Lot No = 709352
Cyl No = 14
Exp Date = 12/23/2011
County = 23 Oper No. = 020828

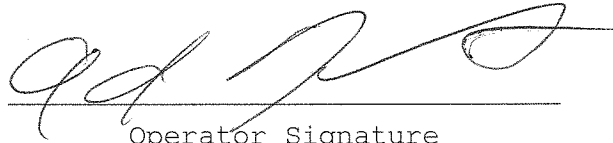

Operator Signature
ADAM R. KRABBENHOFT

Remarks: *ACA TEST*

Form 106-I8000

80-004942
P. 60 of 60
SEM