

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program

Form: BrF-105-G

ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Berry Vanette

Location: Moh L

Intoxilyzer Serial No.: 80-004198

Lot Number: 659358

Cylinder Number: 27

Expiration Date: 9-3-11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 679 %

Test 2: 0. 680 %

Test 3: 0. 679 %

(ATTACH TEST RECORD)

Berry Vanette
Chemical Test Operator Signature

2-2-10
Date

Deb Kashner
Reviewed By

31 Mar 2010
Date

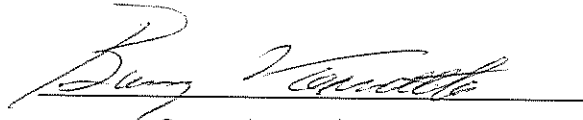
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = MOHL 8164.13.00 06/09
02/02/2010 15:10

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:11
02 Std. Gas	0.079	15:11
03 Room Air	0.000	15:12
04 Std. Gas	0.080	15:12
05 Room Air	0.000	15:13
06 Std. Gas	0.079	15:13
07 Room Air	0.000	15:13

Lot No = 659358
Cyl No = 27
Exp Date = 09/03/2011
County = 38 Oper No. = 039909


Operator Signature
BARRY A. VANNATTA

Remarks:

Form 106-I8000

80-004198
8/31 PM