



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION

Toxicology Section/Breath Alcohol Program

SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Lori Flaten</u>		
Location: <u>Mendon PD</u>		
Intoxilyzer® Serial Number: <u>80-004939</u>		
Gas Lot Number: <u>659358</u>	Gas Cylinder Number: <u>40</u>	Expiration Date: <u>09-03-11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>082</u> %		
Test 2: 0. <u>081</u> %		
Test 3: 0. <u>081</u> %		
(ATTACH TEST RECORD)		

Chemical Test Operator Signature

02-11-11

Date

Reviewed By

15 Feb 2011

Date

80-004939
P. 49 of 50
YFM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = MAND 8164.13.00 06/09
02/11/2011 13:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:42
02 Std. Gas	0.082	13:43
03 Room Air	0.000	13:43
04 Std. Gas	0.081	13:44
05 Room Air	0.000	13:44
06 Std. Gas	0.081	13:45
07 Room Air	0.000	13:45


Lot No = 659358

Cyl No = 40

Exp Date = 09/03/2011

County = 30

Oper No. = 068019

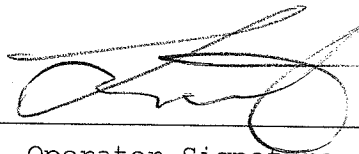

Operator Signature
LORI E. FLATEN

Remarks:

Form 106-I8000

80-004939
P. 50 of 50
JFM