

Intoxilyzer 8000 Initial Inspection

Serial Number	80-004956
----------------------	------------------

A. Power On 5 min. countdown 1 min.

B. Security Checks. Level 1 Level 2 Level 3

C. Gas Cylinder Setup

D. Printer. Level 1 Func P Paper Feed Internal External

E. Display is working.

F. Configure Start Test Switch. Level 3 Func S Sub T

G. Setup Preliminary Data. Level 2 Func E

H. Configure General Setup. Level 3 Func S Sub G.

I. Configure Port. Level 3 Func S Sub N

J. Check Camera. ABA Mode Oper ID ND Lic. Hot Key "R"

K. Diagnostic Test. Level 2 Func D

L. Check Ser Num / Version Level 2 Func V
 80-004956 Serial No. 8164.13 Version 1364.14 Display 7 CPLD

M. Detector Voltages. Level 3 Func D Sub D
 3 12791 s 1 C 47.0
 9 13129 s 3 B 45 0 RFI Ind.

N. Hot Keys
 F5 Tone
 F6 Green LED
 F7 Red LED
 F9 Fan
 F10 Pump
 F11 Sol Output

O. RFI Dectector

P. Atmospheric Monitor. Level 3 Func D Sub A. P 1013 CF 0.99

OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 Instrument Certification and Maintenance Unit

BrF-005-8

<u>✓</u>	Q. Flow Monitor. Level 3 Func D Sub F.	R	<u>229</u>	F	<u>0.00</u>	Us	
<u>✓</u>	R. Temperature Monitor. Level 3 Func D Sub T	C	<u>47.0</u>	A	<u>47.0</u>	I	<u>0.0</u>
		B	<u>44.9</u>	V	<u>0.0</u>		
<u>✓</u>	S. Gas Tank Monitor. Level 3 Func D Sub G		<u>452</u> psi Intox		<u>450</u> psi Reg		
<u>✓</u>	T. Configure Wet Bath Sim. Level 1 Func S						
<u>✓</u>	U. Zero Alcohol Test Level 1 Func C		<u>G10369</u> <u>DR5175</u> Sim SN		— Lot		<u>0.00</u> Rep Value
		mAP	<u>0.000</u> AC		<u>0.000</u> AC		<u>0.000</u> AC
<u>✓</u>	V. Low AC Test. Level 1 Func C		<u>DR5190</u> Sim SN		— Lot		<u>0.021</u> Rep Value
			<u>0.018</u> AC		<u>0.019</u> AC		<u>0.020</u> AC
<u>✓</u>	W. Linearity Test. Level 1 Func C		<u>DR5113</u> Sim SN		— Lot		<u>0.285</u> Rep Value
			<u>0.286</u> AC		<u>0.289</u> AC		<u>0.290</u> AC
<u>✓</u>	X. Interferent Test. Level 1 Func B	Acetone	<u>DR5186</u> Sim SN		— Lot		<u>0.059%</u> Conc
			<u>✓</u> Display		<u>✓</u> Printout		
		Methanol	<u>DR3846</u> Sim SN		— Lot		<u>0.10%</u> Conc
			<u>✓</u> Display		<u>✓</u> Printout		
		IPA	<u>DR3840</u> Sim SN		— Lot		<u>0.10%</u> Conc
			<u>✓</u> Display		<u>✓</u> Printout		
<u>✓</u>	Y. Ambient Test		<u>✓</u> Display		<u>✓</u> Printout		
<u>✓</u>	Z. Invalid Sample Test		<u>✓</u> Display		<u>✓</u> Printout		
<u>✓</u>	AA. RFI Detector Test. CMS Mode		<u>✓</u> Display		<u>✓</u> Printout		
<u>✓</u>	BB. Configure Dry Gas Standard. Level 1 Func S						
<u>✓</u>	CC. Stability Test at 0.080AC. Level 3 Func T Sub S		<u>0.0797</u> Ave.		<u>0.0005</u> Std Dev		<u>0.62</u> Rel Std Dev
<u>✓</u>	DD. Maintenance/Repairs	<u>Calibration - Opt. Bench</u>					

12 February 2010
 Date
~~16 Feb 2010~~ 12 Feb 2010
 Date

Mary Pearson
 Signature
Deb Kasher
 Reviewed by

80-004956
 7/24 KAL

TOXL
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-004956
 02/12/2010 08:21:55

Auto Calibration

	<<<<<	3um	>>>>>	<<<<<	9um	>>>>>

Solution = 0.000 g/210L or 0.0000 mg/l, Samples = 4, Discarded = 1						
Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)		
Sample #1	0.0270	(-0.0020)	0.0470	(0.0180)		
Sample #2	0.0420	(-0.0030)	0.0500	(0.0180)		
Sample #3	0.0250	(0.0080)	0.0290	(0.0160)		
Sample #4	0.0340	(0.0120)	0.0160	(0.0110)		
Avg % Abs	0.0337	(0.0057)	0.0317	(0.0150)		
STD DEV	0.0085	(0.0078)	0.0172	(0.0036)		
REL STD DEV	25.262	(137.073)	54.177	(24.037)		

Solution = 0.021 g/210L or 0.1000 mg/l, Samples = 4, Discarded = 1						
Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)		
Sample #1	0.3780	(-0.0090)	0.7410	(0.0050)		
Sample #2	0.3620	(0.0150)	0.7450	(-0.0090)		
Sample #3	0.3910	(0.0150)	0.7950	(0.0040)		
Sample #4	0.4020	(0.0170)	0.7960	(0.0030)		
Avg % Abs	0.3850	(0.0157)	0.7787	(-0.0007)		
STD DEV	0.0207	(0.0012)	0.0292	(0.0072)		
REL STD DEV	5.367	(7.370)	3.745	(1085.127)		

Solution = 0.041 g/210L or 0.1952 mg/l, Samples = 4, Discarded = 1						
Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)		
Sample #1	0.7750	(-0.0190)	1.5430	(0.0000)		
Sample #2	0.8000	(-0.0100)	1.5880	(-0.0040)		
Sample #3	0.7670	(0.0000)	1.5640	(0.0100)		
Sample #4	0.7840	(0.0060)	1.6110	(-0.0040)		
Avg % Abs	0.7837	(-0.0013)	1.5877	(0.0007)		
STD DEV	0.0165	(0.0081)	0.0235	(0.0081)		
REL STD DEV	2.106	(606.218)	1.480	(1212.436)		

Solution = 0.106 g/210L or 0.5048 mg/l, Samples = 4, Discarded = 1						
Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)		
Sample #1	2.0620	(0.0040)	3.9720	(-0.0190)		
Sample #2	2.0710	(0.0030)	3.9970	(-0.0220)		
Sample #3	2.0420	(0.0160)	3.9890	(-0.0340)		
Sample #4	2.0540	(0.0120)	3.9640	(-0.0060)		
Avg % Abs	2.0557	(0.0103)	3.9833	(-0.0207)		
STD DEV	0.0146	(0.0067)	0.0172	(0.0140)		
REL STD DEV	0.709	(64.435)	0.432	(67.972)		

Solution = 0.285 g/210L or 1.3571 mg/l, Samples = 4, Discarded = 1						
Sample	% Abs	(% Abs Ref)	% Abs	(% Abs Ref)		
Sample #1	5.2640	(-0.0120)	9.8640	(-0.0170)		
Sample #2	5.2580	(0.0200)	9.8880	(-0.0130)		
Sample #3	5.2630	(0.0150)	9.9030	(-0.0030)		
Sample #4	5.2660	(0.0180)	9.8940	(0.0110)		
Avg % Abs	5.2623	(0.0177)	9.8950	(-0.0017)		
STD DEV	0.0040	(0.0025)	0.0075	(0.0121)		
REL STD DEV	0.077	(14.245)	0.076	(723.326)		

80-004956
 5/29 KAL

Calibration
 01/07/12
 MHP

TOXL
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-004956
 02/12/2010 08:21:55

Auto Calibration

pg 2 of 2

<<<<< 3um >>>>>

 Zero Order Coef -3.09
 First Order Coef 2412.49
 Second Order Coef 31.56

<<<<< 9um >>>>>

 0.61
 1202.96
 17.00

Act (g/210L)	Fit (g/210L)	Residual (g/210L)
0.000	0.002	-0.0016
0.021	0.020	0.0015
0.041	0.040	0.0010
0.106	0.107	-0.0009
0.285	0.285	0.0001

Act (g/210L)	Fit (g/210L)	Residual (g/210L)
0.000	0.001	-0.0008
0.021	0.020	0.0011
0.041	0.041	-0.0000
0.106	0.106	-0.0003
0.285	0.285	0.0001

<<<<< 3um >>>>> <<<<< 9um >>>>>

 Solution = 0.080 g/210L or 0.3810 mg/l, Samples = 4, Discarded = 1
 Sample

Sample #1	3297.00	3243.00
Sample #2	3249.00	3281.00
Sample #3	3244.00	3266.00
Sample #4	3269.00	3265.00
Avg	3254.0000	3270.6667
STD DEV	13.2288	8.9629
REL STD DEV	0.407	0.274
H2O adjust (mg/l*10k)	555	539

Atmospheric Pressure = 1015

*****CALIBRATION SUCCESSFUL*****

80-004956
 9/24 KR
 Calibration
 02/12/2010
 MAP

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CM1, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 08:06

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMN

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQRSTU

24 characters per line
abcdefghijklmnopqrstuvw
ABCDEFGHIJKLMNQRSTUW

32 characters per line
abcdefghijklmnopqrstuvwxy123456
ABCDEFGHIJKLMNQRSTUWXYZ123456

42 characters per line
abcdefghijklmnopqrstuvwxy1234567890abcdef
ABCDEFGHIJKLMNQRSTUWXYZ1234567890ABCDEF


Current Instrument Setup
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Menfll? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.000
Standard Lot #? 123456789
Standard Cyl #? 123456
Standard Expiration? 11/11/2011
Oper No? 107501

Flow Cal. Date: 01/25/2010
Slope 672
Intercept -627011

IR Calibration Date: 01/25/2010
3um 9um

0th Coef(*100):	-8483	-22783
1st Coef(*100):	253277	131946
2nd Coef(*100):	1955	961
H2O adj(mg/l)*10k):	518	449

***** Test End *****


Operator Signature
MARGY PEARSON

Remarks:

Print Test

Form 106-18000

80-004956
10/24 PM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 09:22

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMN0PQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 123456789
Standard Cyl #? 123456
Standard Expiration? 11/11/2011
Oper No? 107501

Flow Cal. Date: 01/25/2010
Slope 672
Intercept -627011

IR Calibration Date: 02/12/2010
 3um 9um

0th Coef(*100):	-309	61
1st Coef(*100):	241249	120296
2nd Coef(*100):	3156	1700
H2O adj (mg/l*10k):	555	539

***** Printer Test End *****



Operator Signature
MARGY PEARSON

Remarks:




Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 11:11

Test	AC	Time
01 Room Air	0.000	11:12
02 *Subject Test	REF*	11:12
03 Room Air	0.000	11:12

*Subject Test Refused

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 11/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 668180
Cyl No = 94
Expiration Date = 09/21/2011
County = 08 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

Camera / Refusal "R" key

Form 106-I8000

80-004956
12/24 1972

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 11:14

DIAGNOSTIC

Voltage/Current Test	Pass
RAM Test	Pass
EEPROM Checksum Test	Pass
Real Time Clock Test	Pass
DSP Test	Pass
Analytical Stability Test	Pass
Modem Test	Pass
Temp Regulation Test	Pass

Oper No. = 107501

Margy Pearson

Operator Signature
MARGY PEARSON

Remarks:

DIAGNOSTIC

Form 106-I8000

80-004956
12/24 KR

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 12:11

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:11
02 Std. Sol.	0.000	12:12
03 Room Air	0.000	12:13
04 Std. Sol.	0.000	12:13
05 Room Air	0.000	12:14
06 Std. Sol.	0.000	12:15
07 Room Air	0.000	12:15

08 Sim Temp = 34.0°C

Simul Ser No = 000000

Std Sol No = 0000

County = 08

Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

Z110 0.00 AC

Form 106-I8000

80-004956
14/24 PM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 14:30

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:31
02 Std. Sol.	0.018	14:33
03 Room Air	0.000	14:33
04 Std. Sol.	0.019	14:34
05 Room Air	0.000	14:34
06 Std. Sol.	0.020	14:35
07 Room Air	0.000	14:35

08 Sim Temp = 34.0°C

Simul Ser No = 000000
Std Sol No = 0000
County = 08 Oper No. = 107501

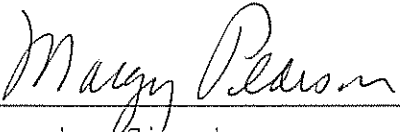

Operator Signature
MARGY PEARSON

Remarks:

Low ~~0.018~~ ^{meP} 0.021 AC

Form 106-I8000

80-004956
1/24 FR

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 14:43

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:43
02 Std. Sol.	0.286	14:44
03 Room Air	0.000	14:45
04 Std. Sol.	0.289	14:46
05 Room Air	0.000	14:46
06 Std. Sol.	0.290	14:47
07 Room Air	0.000	14:48


08 Sim Temp = 34.0°C

Simul Ser No = 000000

Std Sol No = 0000

County = 08

Oper No. = 107501

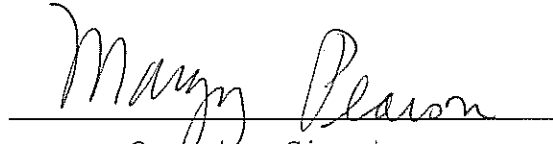

Operator Signature
MARGY PEARSON

Remarks:

Linearity 0.285 AC

Form 106-I8000

80-004956
10/24 PM


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 15:06

Test	AC	Time
01 Room Air	0.000	15:08
02 *Subject Test	INT*	15:08
03 Room Air	0.000	15:08

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 11/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Simul Ser No = 000000
Std Sol No = 0000
County = 08 Oper No. = 107501

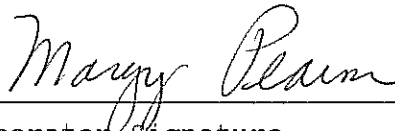

Operator Signature
MARGY PEARSON

Remarks:

Acetone - Interfer

Form 106-I8000

80-004956
17/24 1992

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 15:04

Test	AC	Time
01 Room Air	0.000	15:05
02 *Subject Test	INT*	15:05
03 Room Air	0.000	15:06

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 11/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Simul Ser No = 000000
Std Sol No = 0000
County = 08 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

MeOH Interfer

Form 106-I8000

80-004956
12/24 15:04


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 15:09

Test	AC	Time
01 Room Air	0.000	15:09
02 *Subject Test	INT*	15:10
03 Room Air	0.000	15:10

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 11/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Simul Ser No = 000000
Std Sol No = 0000
County = 08 Oper No. = 107501

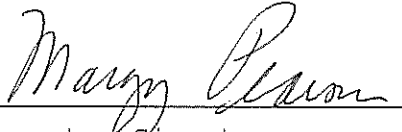

Operator Signature
MARGY PEARSON

Remarks:

IPA Interfer

Form 106-I8000

80-004956
12/24 174


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 15:13

Test	AC	Time
01 Room Air	AMB*	15:16
02 Room Air	0.000	15:16

*Invalid Test
Check Ambient Conditions

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 11/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 668180
Cyl No = 94
Expiration Date = 09/21/2011
County = 08 Oper No. = 107501



Operator Signature
MARGY PEARSON

Remarks:

Ambient

Form 106-I8000

80-004956
2/24/14


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 15:17

Test	AC	Time
01 Room Air	0.000	15:17
02 Invalid Sample	X.XXX	15:18
03 Room Air	0.000	15:18

*Invalid Test - Mouth Alcohol

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 11/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 668180
Cyl No = 94
Expiration Date = 09/21/2011
County = 08 Oper No. = 107501

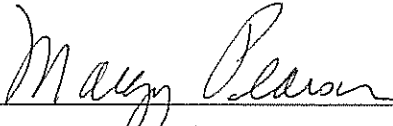

Operator Signature
MARGY PEARSON

Remarks:

Invalid Sample

Form 106-I8000

80-004956
2/24 YFA

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 15:01

Test	AC	Time
01 Diagnostic	OK	15:02
02 Room Air	RFI*	15:02
03 Room Air	0.000	15:03

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 11/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Simul Ser No = 000000
Std Sol No = 0000
County = 08 Oper No. = 107501

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
MARGY PEARSON

Remarks:

RFI

Form 106-I8000

80-004956
2/14 YR

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004956
Location = TOXL 8164.13.00 06/09
02/12/2010 09:32

Test	AC	Time
01 Room Air	0.000	09:32
02 Std. Gas	0.079	09:33
03 Room Air	0.000	09:33
04 Std. Gas	0.080	09:34
05 Room Air	0.000	09:34
06 Std. Gas	0.079	09:35
07 Room Air	0.000	09:35
08 Std. Gas	0.079	09:35
09 Room Air	0.000	09:36
10 Std. Gas	0.080	09:36
11 Room Air	0.000	09:37
12 Std. Gas	0.079	09:37
13 Room Air	0.000	09:38
14 Std. Gas	0.080	09:38
15 Room Air	0.000	09:38
16 Std. Gas	0.079	09:39
17 Room Air	0.000	09:39
18 Std. Gas	0.080	09:40
19 Room Air	0.000	09:40
20 Std. Gas	0.080	09:41
21 Room Air	0.000	09:41
22 Std. Gas	0.080	09:41
23 Room Air	0.000	09:42
24 Std. Gas	0.080	09:42
25 Room Air	0.000	09:43
26 Std. Gas	0.079	09:43
27 Room Air	0.000	09:44
28 Std. Gas	0.080	09:44
29 Room Air	0.000	09:44
30 Std. Gas	0.080	09:45
31 Room Air	0.000	09:45
32 Std. Gas	0.079	09:46
33 Room Air	0.000	09:46
34 Std. Gas	0.080	09:47
35 Room Air	0.000	09:47
36 Std. Gas	0.080	09:47
37 Room Air	0.000	09:48
38 Std. Gas	0.080	09:48
39 Room Air	0.000	09:49
40 Std. Gas	0.080	09:49
41 Room Air	0.000	09:50
42 Cal Check Stats:		
43 Average	0.0797	
44 Std Dev	0.0005	
45 Rel Std Dev	0.62%	

Stability Test
P1062
MAP

80-004956
23/54 AK

Operator Signature
MARGY PEARSON

Remarks:

Form 106-I8000

LOT 668180
Cyl. 94
Exp date 9/21/2011

Stability Test
p 2 of 2
MAP

80-604956
24/24 1574