



ETHANOL BREATH STANDARD CYLINDER REPORT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>D. OLDENBURG -274</u>		
Location: <u>WALSH CO. LEC GRAPTON, ND</u>		
Intoxilyzer® Serial Number: <u>80-002666</u>		
Gas Lot Number: <u>059358</u>	Gas Cylinder Number: <u>16</u>	Expiration Date: <u>09/03/11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.079</u> %		
Test 2: <u>0.079</u> %		
Test 3: <u>0.080</u> %		
(ATTACH TEST RECORD)		

D. Oldenburg 274
 Chemical Test Operator Signature

02/17/11 02/17/11 DK
 Date

Deb Kashur
 Reviewed By

22 Feb 2011
 Date

80-002666
 P. 76 of 77
 FM

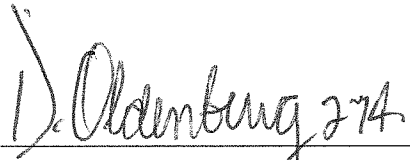
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-002666
Location = GRAF 8164.13.00 06/09
02/17/2011 08:21

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	08:22
02 Std. Gas	0.079	08:22
03 Room Air	0.000	08:23
04 Std. Gas	0.079	08:23
05 Room Air	0.000	08:24
06 Std. Gas	0.080	08:24
07 Room Air	0.000	08:24

Lot No = 659358
Cyl No = 16
Exp Date = 09/03/2011
County = 50 Oper No. = 048915


Operator Signature
DOLF OLDENBURG

Remarks:

Form 106-I8000

80-002666
P-77-477
FM