



**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
 OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION  
 Toxicology Section/Breath Alcohol Program  
 SFN 59281 (5-2011)

|   |   |
|---|---|
| Serial Number<br><i>80-005362</i>   | Instrument Location<br><i>Cooperstown</i> |
| Reason for Install/Repair<br><input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change<br><input type="checkbox"/> Other (Specify) _____ |   |

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. RFI Test (Use CMS Mode; Key Radio During First Room Air).
- 7. Repair and/or Maintenance Performed (if Any): *None*
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

|  |                          |
|--|--------------------------|
| Field Inspector Signature<br><i>[Signature]</i>              | Date<br><i>2/22/13</i>   |
| Reviewed By (Crime Laboratory Use Only)<br><i>Deb Kashur</i> | Date<br><i>25 Feb 13</i> |




Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005362  
Location = COOP                    8164.13.00 06/09  
02/22/2013                            13:53

DRY CAL CHECK

| Test        | AC    | Time  |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 13:54 |
| 02 Std. Gas | 0.084 | 13:54 |
| 03 Room Air | 0.000 | 13:55 |
| 04 Std. Gas | 0.083 | 13:55 |
| 05 Room Air | 0.000 | 13:56 |
| 06 Std. Gas | 0.083 | 13:56 |
| 07 Room Air | 0.000 | 13:57 |

Lot No = 16512080A2  
Cyl No = 30  
Exp Date = 08/01/2014  
County = 20                            Oper No. = 011017



Operator Signature  
JUSTIN WALLERICH

Remarks:

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-005362  
Location = COOP                    8164.13.00 06/09  
02/22/2013                            14:01

| Test          | AC    | Time  |
|---------------|-------|-------|
| 01 Diagnostic | OK    | 14:02 |
| 02 Room Air   | RFI*  | 14:03 |
| 03 Room Air   | 0.000 | 14:03 |

\*Invalid Test  
Inhibited - RFI

Sub Name = TEST, NA NA  
Sub DOB = 11/12/1994  
Sub Sex = Male                    Weight = 200  
Test = DUI                        Cit = 00000  
Dr. Lic. = ND/NA  
Lot No = 16512080A2  
Cyl No = 30  
Expiration Date = 08/01/2014  
County = 20                        Oper No. = 011017

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

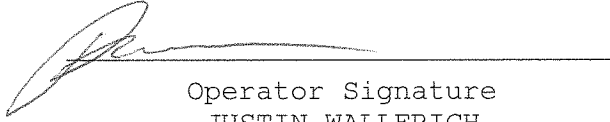  
Operator Signature  
JUSTIN WALLERICH

Remarks:

Form 106-I8000