


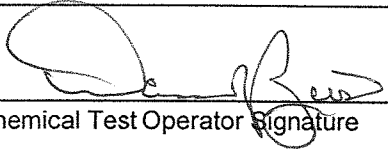

**ETHANOL BREATH STANDARD CYLINDER REPORT**  
OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name:	DAVID J. ZEIS				
Location:	CAVALIER County Sheriff's Office - Langdon				
Intoxilyzer® Serial Number:	80-004937				
Gas Lot Number:	659358	Gas Cylinder Number:	22	Expiration Date:	09/03/2011
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed				
Instrument Test Results (Report to 3 Digits; Example, 0.081%)					
Test 1: 0.079 %					
Test 2: 0.080 %					
Test 3: 0.079 %					
(ATTACH TEST RECORD)					

  
\_\_\_\_\_  
Chemical Test Operator Signature

02/24/2011  
\_\_\_\_\_  
Date

Deb Kashur  
\_\_\_\_\_  
Reviewed By

01 Mar 2011  
\_\_\_\_\_  
Date

80-004937  
p. 56 of 57  
AM


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004937  
Location = LANG                    8164.13.00 06/09  
02/24/2011                            15:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:47
02 Std. Gas	0.079	15:47
03 Room Air	0.000	15:48
04 Std. Gas	0.080	15:48
05 Room Air	0.000	15:49
06 Std. Gas	0.079	15:49
07 Room Air	0.000	15:49

Lot No = 659358  
Cyl No = 22  
Exp Date = 09/03/2011  
County = 10                            Oper No. = 067518

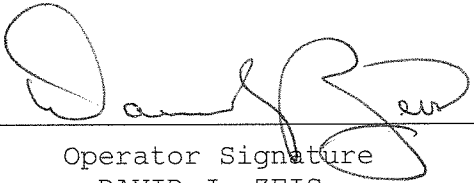  
Operator Signature  
DAVID J. ZEIS

Remarks:

Form 106-I8000

80-004937  
P. 57 of 57  
FM