

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program

Form: BrF-105-G

### ETHANOL BREATH STANDARD CYLINDER REPORT

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Jonathan Tofield

Location: Mohall

Intoxilyzer Serial No.: 80-004198

Lot Number: 659358

Cylinder Number: 27

Expiration Date: 9/3/011

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 079 %

Test 2: 0. 078 %

Test 3: 0. 078 %

(ATTACH TEST RECORD)

[Signature]  
Chemical Test Operator Signature

3-11-10 <sup>DK</sup> 3-02-10  
Date

Deb Kashner  
Reviewed By

11 Mar 2010  
Date

80-004198  
P.1 of 2 rev

75/16

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004198  
Location = MOHL      8164.13.00 06/09  
03/02/2010      13:34

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:35
02 Std. Gas	0.079	13:35
03 Room Air	0.000	13:35
04 Std. Gas	0.078	13:36
05 Room Air	0.000	13:36
06 Std. Gas	0.078	13:37
07 Room Air	0.000	13:37


Lot No = 659358

Cyl No = 27

Exp Date = 09/03/2011

County = 38

Oper No. = 100915

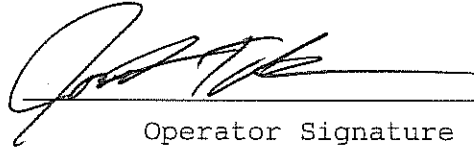

Operator Signature  
JONATHAN TOFTELAND

Remarks:

Form 106-18000

80-004198  
P. 2 of 2 ycm  
76/76