

ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION

Toxicology Section/Breath Alcohol Program

SFN 59262 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Hinton, Rick</u>			
Location: <u>Cass County Jail</u>			
Intoxilyzer @ Serial Number: <u>80-004205</u>			
Lot Number: <u>659357</u>	Cylinder Number: <u>40</u>	Expiration Date: <u>9-3-11</u>	
<input type="checkbox"/> New Cylinder Installed		<input checked="" type="checkbox"/> Cylinder not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)			
Test 1: 0. <u>83</u> %			
Test 2: 0. <u>83</u> %			
Test 3: 0. <u>83</u> %			
(ATTACH TEST RECORD)			

3554
 Chemical Test Operator Signature

3-2-10
 Date

Deb Kashner
 Reviewed By

10 May 2010
 Date

80-004205
 P. 46/67 sam

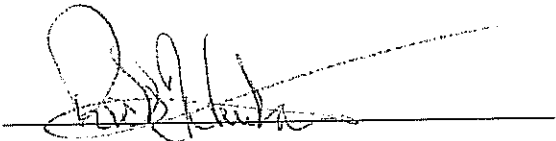
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004205
Location = CASS 8164.13.00 06/09
03/02/2010 15:36

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:37
02 Std. Gas	0.083	15:38
03 Room Air	0.000	15:38
04 Std. Gas	0.083	15:38
05 Room Air	0.000	15:39
06 Std. Gas	0.083	15:39
07 Room Air	0.000	15:40

Lot No = 659357
Cyl No = 40
Exp Date = 09/03/2011
County = 09 Oper No. = 029920


Operator Signature
RICK HINTON

Remarks:

Form 106-I8000

80-004205
P. 2 of 2
07/16/11