



ETHANOL BREATH STANDARD CYLINDER REPORT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Chris Pulver</u>		
Location: <u>Mountail SD</u>		
Intoxilyzer® Serial Number: <u>80-004943</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>34</u>	Expiration Date: <u>12-23-11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: 0. <u>080</u> % Test 2: 0. <u>079</u> % Test 3: 0. <u>080</u> %		
(ATTACH TEST RECORD)		

Chris Pulver
 Chemical Test Operator Signature

3-5-11
 Date

Deb Kashner
 Reviewed By

23 Mar 2011
 Date

80-004943
 P. 63 of 24
 YFM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004943
Location = STAN 8164.13.00 06/09
03/05/2011 22:59

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	23:00
02 Std. Gas	0.080	23:01
03 Room Air	0.000	23:01
04 Std. Gas	0.079	23:01
05 Room Air	0.000	23:02
06 Std. Gas	0.080	23:02
07 Room Air	0.000	23:03


Lot No = 709352

Cyl No = 34

Exp Date = 12/23/2011

County = 31

Oper No. = 049912

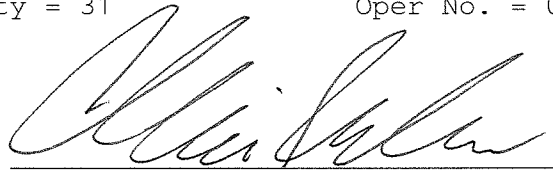

Operator Signature
CHRISTOPHER PULVER

Remarks:

Form 106-I8000

80-004943
P. 64 of 64
vsm