



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION

Toxicology Section/Breath Alcohol Program

SFN 59281 (5-2011)

Serial Number 80-004950	Instrument Location Williams Co LEC
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. RFI Test (Use CMS Mode; Key Radio During First Room Air).
- 7. Repair and/or Maintenance Performed (if Any): N/A
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>Scenie M. Hurdell</i>	Date 08 March 2013 ✓
Reviewed By (Crime Laboratory Use Only) <i>Deb Kasher</i>	Date 26 Mar 2014

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = WILL 8164.13.00 06/09
03/08/2013 20:49

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxy1234567890-|=|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

Current Instrument Setup

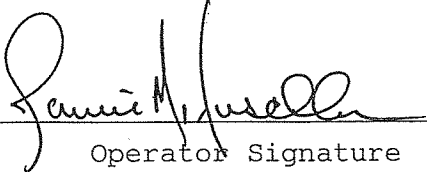
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 23411080A1
Standard Cyl #? 50
Standard Expiration? 10/01/2013
Oper No? 100406

Flow Cal. Date: 01/18/2010
Slope 774
Intercept -908904

IR Calibration Date: 04/06/2011
 3um 9um

0th Coef(*100): -2573 -7967
1st Coef(*100): 257525 132746
2nd Coef(*100): 5623 2169
H2O adj(mg/l*10k): 540 597

***** Printer Test End *****


Operator Signature
JAMIE HUSCHKA

Remarks:

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = WILL 8164.13.00 06/09
03/08/2013 20:45

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	20:46
02 Std. Gas	0.079	20:46
03 Room Air	0.000	20:47
04 Std. Gas	0.080	20:47
05 Room Air	0.000	20:47
06 Std. Gas	0.081	20:48
07 Room Air	0.000	20:48

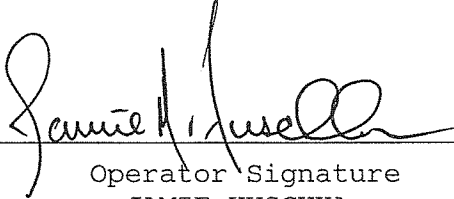
Lot No = 23411080A1

Cyl No = 50

Exp Date = 10/01/2013

County = 53

Oper No. = 100406


Operator Signature
JAMIE HUSCHKA

Remarks:

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

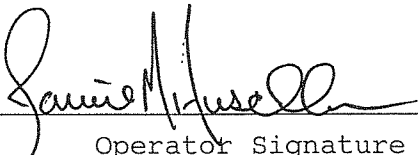
CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = WILL 8164.13.00 06/09
03/08/2013 20:49

DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	20:50
02 Room Air	0.000	20:50

*Invalid Test
Inhibited - RFI

Lot No = 23411080A1
Cyl No = 50
Exp Date = 10/01/2013
County = 53 Oper No. = 100406


Operator Signature
JAMIE HUSCHKA

Remarks:

26 March 2014

Trooper Jamie Huschka did not run the RFI test in CMS mode during his 3-08-2013 Intoxilyzer 8000 installation. However, this does not make the installation ineffective or incomplete. The RFI test Trooper Huschka performed shows that the RFI is working properly on this instrument.

Deb Kashur,



Forensic Scientist,

ND Crime Laboratory