



ETHANOL BREATH STANDARD CYLINDER REPORT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Joe Knowski</u>		
Location: <u>Devils Lake LEC</u>		
Intoxilyzer® Serial Number: <u>80-004193</u>		
Gas Lot Number: <u>15410080A1</u>	Gas Cylinder Number: <u>17</u>	Expiration Date: <u>7-1-2012</u>
<input type="checkbox"/> New Cylinder Installed	<input type="checkbox"/> Cylinder Not Changed	<u>ACA</u>
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.079</u> %		
Test 2: <u>0.079</u> %		
Test 3: <u>0.079</u> %		
(ATTACH TEST RECORD)		

Joe Knowski
 Chemical Test Operator Signature

3-19-2011
 Date

Deb Kashur
 Reviewed By

23 May 2011
 Date

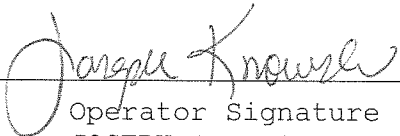
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = DEVL 8164.13.00 06/09
03/19/2011 23:46

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	23:47
02 Std. Gas	0.079	23:47
03 Room Air	0.000	23:48
04 Std. Gas	0.079	23:48
05 Room Air	0.000	23:48
06 Std. Gas	0.079	23:49
07 Room Air	0.000	23:49

Lot No = ~~659358~~ 15410080A1 DK
Cyl No = ~~20~~ 17
Exp Date = ~~09/03/2011~~ 07/01/2012
County = 36 Oper No. = 109208


Operator Signature
JOSEPH J. KNOWSKI

Remarks:

Form 106-I8000

80-004193
p. 95 of 95
FM