



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

| | | |
|---|---|--------------------------------|
| Chemical Test Operator Name: <u>Sean Murphy</u> | | |
| Location: <u>Battineau County Sheriff's Dept.</u> | | |
| Intoxilyzer® Serial Number: <u>80-003065</u> | | |
| Gas Lot Number: <u>05911080A1</u> | Gas Cylinder Number: <u>19</u> | Expiration Date: <u>2-1-13</u> |
| <input checked="" type="checkbox"/> New Cylinder Installed | <input type="checkbox"/> Cylinder Not Changed | |
| Instrument Test Results (Report to 3 Digits; Example, 0.081%) | | |
| Test 1: <u>0.079</u> % | | |
| Test 2: <u>0.079</u> % | | |
| Test 3: <u>0.078</u> % | | |
| (ATTACH TEST RECORD) | | |

[Signature]
Chemical Test Operator Signature

9-8-11
Date

Deb Kashner
Reviewed By

02 Apr 2012
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003065
Location = BOTT 8164.13.00 06/09
09/08/2011 15:18

DRY CAL CHECK

| Test | AC | Time |
|-------------|-------|-------|
| 01 Room Air | 0.000 | 15:19 |
| 02 Std. Gas | 0.079 | 15:19 |
| 03 Room Air | 0.000 | 15:20 |
| 04 Std. Gas | 0.079 | 15:20 |
| 05 Room Air | 0.000 | 15:21 |
| 06 Std. Gas | 0.078 | 15:21 |
| 07 Room Air | 0.000 | 15:22 |

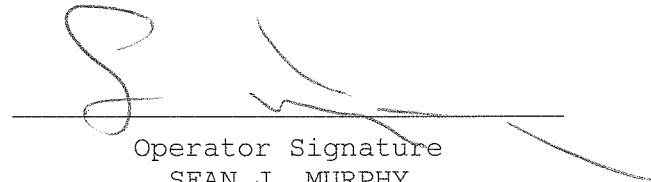
Lot No = 05911080A1

Cyl No = 19

Exp Date = 02/01/2013

County = 05

Oper No. = 039117


Operator Signature
SEAN J. MURPHY

Remarks:

Form 106-I8000