



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION

Toxicology Section/Breath Alcohol Program

SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Rude, Josh</u>		
Location: <u>Stutsman Co.</u>		
Intoxilyzer® Serial Number: <u>80-004198</u>		
Gas Lot Number: <u>0591080A1</u>	Gas Cylinder Number: <u>21</u>	Expiration Date: <u>2-6-13</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.077</u> %		
Test 2: <u>0.078</u> %		
Test 3: <u>0.078</u> %		
(ATTACH TEST RECORD)		

[Signature]
Chemical Test Operator Signature

8-18-11
Date

Deb Kashner
Reviewed By

03 Apr 12
Date

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = JAME 8164.13.00 06/09
08/18/2011 10:49

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:50
02 Std. Gas	0.077	10:50
03 Room Air	0.000	10:51
04 Std. Gas	0.078	10:51
05 Room Air	0.000	10:52
06 Std. Gas	0.078	10:52
07 Room Air	0.000	10:53

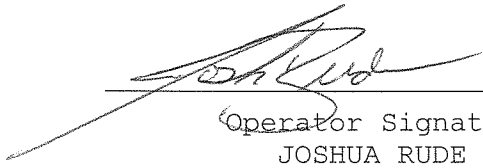
Lot No = 05911080A1

Cyl No = 21

Exp Date = 02/01/2013

County = 47

Oper No. = 100414


Operator Signature
JOSHUA RUDE

Remarks: