



ETHANOL BREATH STANDARD CYLINDER REPORT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Chris Pulver</u>		
Location: <u>Mountrail 50</u>		
Intoxilyzer® Serial Number: <u>80-004943</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>34</u>	Expiration Date: <u>12-23-11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: <u>0.079</u> % Test 2: <u>0.080</u> % Test 3: <u>0.080</u> %		
(ATTACH TEST RECORD)		

Chris Pulver
 Chemical Test Operator Signature

4-15-11
 Date

Deb Kashner
 Reviewed By

19 Apr 11
 Date


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004943
Location = STAN 8164.13.00 06/09
04/15/2011 15:57

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:58
02 Std. Gas	0.079	15:58
03 Room Air	0.000	15:59
04 Std. Gas	0.080	15:59
05 Room Air	0.000	16:00
06 Std. Gas	0.080	16:00
07 Room Air	0.000	16:01

Lot No = 709352
Cyl No = 34
Exp Date = 12/23/2011
County = 31 Oper No. = 049912

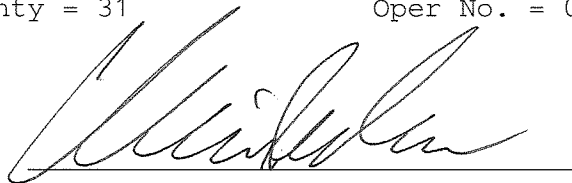

Operator Signature
CHRISTOPHER PULVER

Remarks:

Form 106-I8000

80-004943
P-81281
FM