

INTOXILYZER 8000 INSPECTION

Serial No.: 80-004943

Location: TOX LAB

- |   | Check When Done |
|---|-----------------|
| A. Is the warm-up time less than 20 minutes?  | <u>✓</u>        |
| B. Is a three-pronged grounded outlet used?   | <u>✓</u>        |
| C. Is the breath tube heated?   | <u>✓</u>        |
| D. Is the diagnostic check complete?  | <u>✓</u>        |
| E. Is the time, date, and year correct (re-set if necessary)?   | <u>✓</u>        |
| F. Print test. (Attach test record.)  | <u>✓</u>        |
| G. Low AC. Use <0.03 AC in ACA mode. (Attach test record.)<br>Sim SN <u>DR5140</u> Lot No. <u>—</u> Rep AC <u>0.019 AC</u>  | <u>✓</u>        |
| H. Linearity Test. Use ≥ 0.25 AC in ACA mode. (Attach test record.)<br>Sim SN <u>DR5113</u> Lot No. <u>—</u> Rep AC <u>0.285 AC</u>   | <u>✓</u>        |
| I. Interferent check. Use 0.05% acetone plus 0.10 AC ethanol in ABA mode.<br>(Attach test record.)<br>Sim SN <u>DR5135</u> Lot No. <u>—</u> Rep AC <u>0.10 AC + Acetone</u> | <u>✓</u>        |
| J. RFI check. Run CMS mode. Key radio on first room air.<br>(Attach test record.)   | <u>✓</u>        |
| K. Calibration Check. Use Ethanol Breath Standard cylinder. Do three sets in ACA mode.<br>(Attach test record.)   |                 |

Lot No. <u>709352</u>	Cyl No. <u>34</u>	Exp. Date <u>12/23/2011</u>
Test 1 <u>0.082</u>	Test 4 <u>0.082</u>	Test 7 <u>0.082</u>
Test 2 <u>0.081</u>	Test 5 <u>0.081</u>	Test 8 <u>0.081</u>
Test 3 <u>0.082</u>	Test 6 <u>0.081</u>	Test 9 <u>0.082</u>
Average <u>0.082</u>		

- L. Tank pressure, Level 3 Func D Sub G      P: ~~990~~ <sup>816 MAP</sup> psi Reg ~~850~~ <sup>800 MAP</sup> psi
- M. Remarks/Maintenance record: Annual Inspection, Changed Regulator  
16 April 2010      Mary Pearson  
Date      Field Inspector's Signature  
19 Apr 2010      Deb Kashner  
Date      Reviewed by

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004943  
Location = TOXL                    8164.13.00 06/09  
04/16/2010    13:41

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#%^&\*()\_+?

Current Instrument Setup


Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        No  
# of Print Copies?          1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            709352  
Standard Cyl #?            34  
Standard Expiration?       12/23/2011  
Oper No?                    107501

Flow Cal. Date:            01/18/2010  
Slope                      693  
Intercept                  -665387

IR Calibration Date:       01/18/2010

	3um	9um
0th Coef(*100):	-20351	-24446
1st Coef(*100):	248542	131200
2nd Coef(*100):	2180	1190
H2O adj(mg/l*10k):	594	450

\*\*\*\*\* Printer Test End \*\*\*\*\*

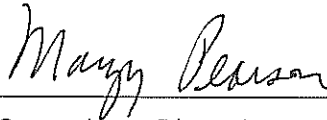

Operator Signature  
MARGY PEARSON

Remarks:

*Print*

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004943  
Location = TOXL      8164.13.00 06/09  
04/16/2010      14:14

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:14
02 Std. Sol.	0.015	14:17
03 Room Air	0.000	14:17
04 Std. Sol.	0.016	14:18
05 Room Air	0.000	14:18
06 Std. Sol.	0.017	14:19
07 Room Air	0.000	14:20


08 Sim Temp = 34.0°C

Simul Ser No = 000000

Std Sol No = 0000

County = 08

Oper No. = 107501



Operator Signature  
MARGY PEARSON

Remarks:

LOW AC 0.019 AC

Form 106-I8000

80-004943  
3/1/10 PA

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004943  
Location = TOXL      8164.13.00 06/09  
04/16/2010      14:20

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:21
02 Std. Sol.	0.281	14:22
03 Room Air	0.000	14:23
04 Std. Sol.	0.286	14:23
05 Room Air	0.000	14:24
06 Std. Sol.	0.286	14:25
07 Room Air	0.000	14:25

08 Sim Temp = 34.0°C

Simul Ser No = 000000

Std Sol No = 0000

County = 08

Oper No. = 107501



Operator Signature  
MARGY PEARSON

Remarks:

Linearity 0.285AC

Form 106-I8000

80-004943  
3/5/90 RM


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004943  
Location = TOXL                8164.13.00 06/09  
04/16/2010                        14:04

Test	AC	Time
01 Room Air	0.000	14:05
02 *Subject Test	INT*	14:05
03 Room Air	0.000	14:06

\*Invalid Test  
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                Weight = 150  
Test = DUI                        Cit = NA  
Dr. Lic. = ND/DIS821456  
Lot No = 709352  
Cyl No = 34  
Expiration Date = 12/23/2011  
County = 08                        Oper No. = 107501



Operator/Signature  
MARGY PEARSON

Remarks:

0.10 AC + 0.05% Acetone

Form 106-I8000

80-004943  
3/10 KAK

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-004943  
Location = TOXL                8164.13.00 06/09  
04/16/2010                        14:30

Test	AC	Time
01 Diagnostic	OK	14:31
02 Room Air	RFI*	14:31
03 Room Air	0.000	14:31

\*Invalid Test  
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT  
Sub DOB = 01/01/1982  
Sub Sex = Female                Weight = 150  
Test = DUI                        Cit = NA  
Dr. Lic. = ND/DIS821456  
Simul Ser No = 000000  
Std Sol No = 0000  
County = 08                        Oper No. = 107501

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature  
MARGY PEARSON

Remarks:

RFI

Form 106-I8000

80-004943  
37/10 VFA


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004943  
Location = TOXL      8164.13.00 06/09  
04/16/2010      13:42

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:43
02 Std. Gas	0.082	13:44
03 Room Air	0.000	13:44
04 Std. Gas	0.081	13:45
05 Room Air	0.000	13:45
06 Std. Gas	0.082	13:45
07 Room Air	0.000	13:46

Lot No = 709352  
Cyl No = 34  
Exp Date = 12/23/2011  
County = 08      Oper No. = 107501



Operator Signature  
MARGY PEARSON

Remarks:

*Cal Check*

Form 106-I8000

80-004943  
3/9/10 *PM*


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004943  
Location = TOXL      8164.13.00 06/09  
04/16/2010      13:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:50
02 Std. Gas	0.082	13:50
03 Room Air	0.000	13:51
04 Std. Gas	0.081	13:51
05 Room Air	0.000	13:52
06 Std. Gas	0.081	13:52
07 Room Air	0.000	13:52

Lot No = 709352  
Cyl No = 34  
Exp Date = 12/23/2011  
County = 08      Oper No. = 107501

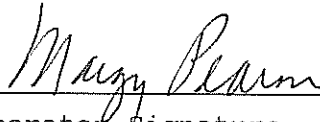

Operator Signature  
MARGY PEARSON

Remarks:

*Cal Check*

Form 106-I8000

80-004943  
39/40 FM



Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004943  
Location = TOXL      8164.13.00 06/09  
04/16/2010      13:54

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:55
02 Std. Gas	0.082	13:55
03 Room Air	0.000	13:56
04 Std. Gas	0.081	13:56
05 Room Air	0.000	13:57
06 Std. Gas	0.082	13:57
07 Room Air	0.000	13:57

Lot No = 709352  
Cyl No = 34  
Exp Date = 12/23/2011  
County = 08      Oper No. = 107501

*Margy Pearson*

Operator Signature  
MARGY PEARSON

Remarks:

*Cal Check*

Form 106-I8000

80-004943  
2/10/40 JAM