



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>JEREMY T. GANDRUD</u>		
Location: <u>BURK</u>		
Intoxilyzer® Serial Number: <u>80-004950</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>2</u>	Expiration Date: <u>12-23-2011</u>
<input checked="" type="checkbox"/> New Cylinder Installed	<input type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>078</u> %		
Test 2: 0. <u>079</u> %		
Test 3: 0. <u>077</u> %		
(ATTACH TEST RECORD)		

[Signature]
Chemical Test Operator Signature

4-23-2010 DK
4-21-2010
Date

Deb Kashur
Reviewed By

10 May 2010
Date

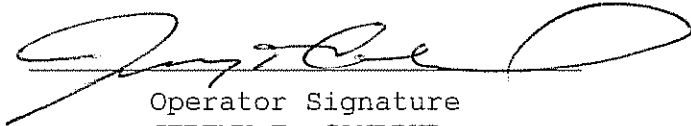
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = BURK 8164.13.00 06/09
04/23/2010 13:30

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:31
02 Std. Gas	0.078	13:31
03 Room Air	0.000	13:32
04 Std. Gas	0.079	13:32
05 Room Air	0.000	13:32
06 Std. Gas	0.077	13:33
07 Room Air	0.000	13:33

Lot No = 709352
Cyl No = 2
Exp Date = 12/23/2011
County = 07 Oper No. = 049303


Operator Signature
JEREMY T. GANDRUD

Remarks:

Form 106-I8000

80-004950
P. 44/44 FM