



# ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Aaron Hummel</u>		
Location: <u>GFSO</u>		
Intoxilyzer® Serial Number: <u>80-004205</u>		
Gas Lot Number: <u>15410080A1</u>	Gas Cylinder Number: <u>23</u>	Expiration Date: <u>2/1/12</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>079</u> %		
Test 2: 0. <u>079</u> %		
Test 3: 0. <u>079</u> %		
(ATTACH TEST RECORD)		

[Signature]  
Chemical Test Operator Signature

5/5/11  
Date

Deb Keshun  
Reviewed By

16 May 2011  
Date

80-004205  
p 110 of 112  
KM


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004205  
Location = GFSO      8164.13.00 06/09  
05/05/2011      13:56

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:56
02 Std. Gas	0.079	13:57
03 Room Air	0.000	13:57
04 Std. Gas	0.079	13:58
05 Room Air	0.000	13:58
06 Std. Gas	0.079	13:58
07 Room Air	0.000	13:59

Lot No = 15410080A1  
Cyl No = 23  
Exp Date = 07/01/2012  
County = 18      Oper No. = 049907

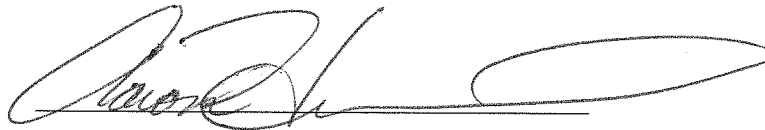

Operator Signature  
AARON HUMMEL

Remarks:

ACA

Form 106-I8000

80-004205  
P. 112 of 112  
KM