



**INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT**  
 OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION  
 Toxicology Section/Breath Alcohol Program  
 SFN 59281 (03-2014)

Serial Number <b>80 006490</b>	Instrument Location <b>TIOGA</b>
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): NONE
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>[Signature]</i> <b>DUISEN SHAWSON</b>	Date <b>5-3-16</b>
Reviewed By (Crime Laboratory Use Only) <i>[Signature]</i> <b>Dub Shanover</b>	Date <b>05 May 16</b>

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006490  
Location = TIOG                    8164.13.00 06/09  
05/03/2016                            12:57

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&\*()\_+?

Current Instrument Setup


Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        Yes  
# of Print Copies?         1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            19615080A5  
Standard Cyl #?            13  
Standard Expiration?       09/05/2017  
Oper No?                    020632

Flow Cal. Date:            08/18/2015  
Slope                      675  
Intercept                  -635799

IR Calibration Date:       08/18/2015  
                                  3um                    9um

-----  
0th Coef(\*100):        -18073                -15729  
1st Coef(\*100):        265337                133887  
2nd Coef(\*100):        3965                    1560  
H2O adj(mg/l\*10k):    767                    457

\*\*\*\*\* Printer Test End \*\*\*\*\*

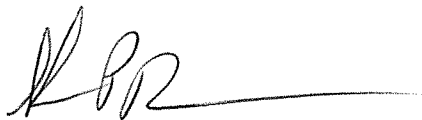

Operator Signature  
SHANNON DUISEN

Remarks:

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006490  
Location = TIOG                    8164.13.00 06/09  
05/03/2016                            12:58

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	12:59
02 Std. Gas	0.080	12:59
03 Room Air	0.000	13:00
04 Std. Gas	0.080	13:00
05 Room Air	0.000	13:00
06 Std. Gas	0.080	13:01
07 Room Air	0.000	13:01

Lot No = 19615080A5  
Cyl No = 13  
Exp Date = 09/05/2017  
County = 53                            Oper No. = 020632



Operator Signature  
SHANNON DUISEN

Remarks:

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006490  
Location = TIOG                8164.13.00 06/09  
05/03/2016                        13:05

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:06
02 Std. Gas	0.080	13:07
03 Room Air	0.000	13:07
04 Std. Gas	RFI*	13:07
05 Room Air	0.000	13:08

\*Invalid Test  
Inhibited - RFI

Lot No = 19615080A5  
Cyl No = 13  
Exp Date = 09/05/2017  
County = 53                      Oper No. = 020632

  
\_\_\_\_\_  
Operator Signature  
SHANNON DUISEN

Remarks: