



# INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION

Toxicology Section/Breath Alcohol Program

SFN 59281 (1-2010)

Serial Number: <u>80-003067</u>	Instrument Location: <u>Redcourt Police Dept</u>
Reason for Install/Repair:	
<input checked="" type="checkbox"/> Install After Lab Repair/Inspection <input type="checkbox"/> Other (Specify) _____	

### Check When Done:

- A. Surge Protector Installed/Properly Grounded.
- B. Telephone Line Connected to Intoxilyzer® 8000.
- C. Breath Tube Heated.
- D. Review/Enter Preliminary Data Entry (Level 2, Function E).
- E. Review/Enter Gas Setup (Level1, Function S).
- F. Print Test (Level 1, Function P). (Attach Test Record.)
- G. ACA Test (Level 1, Function C). (Attach Test Record.)
- H. RFI Test (Use CMS Mode-First Room Air). (Attach Test Record.)
- I. Repair and/or Maintenance Performed: \_\_\_\_\_

[Signature]  
Field Inspector Signature

5-6-2011  
Date

Deb Kashur  
Reviewed By

09 June 2011  
Date

*Install Page # 3*

80-003067  
P. 95 of 98  
KM

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-003067  
Location = BELC      8164.13.00 06/09  
05/06/2011      16:36

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890-=\_|  
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#%^&\*()\_+?

Current Instrument Setup

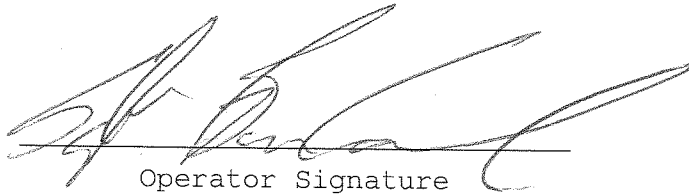
Data Entry Mode: Enabled  
Start Test Sequence: DABACABA  
Display Prelim Rslt? Yes  
Display Third Digit? Yes  
Inhib Printer(Y/N)? No  
Display Volume? No  
Disable On Memfull? Yes  
# of Print Copies? 1  
Select Std (D/W/I)? Dry  
Standard Value? 0.105  
Standard Lot #? 659357  
Standard Cyl #? 38  
Standard Expiration? 09/03/2011  
Oper No? 119802

Flow Cal. Date: 04/08/2008  
Slope 679  
Intercept -607413

IR Calibration Date: 05/03/2011

	3um	9um
0th Coef(*100):	-10062	-6838
1st Coef(*100):	267436	137304
2nd Coef(*100):	3888	1253
H2O adj(mg/l*10k):	530	414

\*\*\*\*\* Printer Test End \*\*\*\*\*



Operator Signature  
BRIAN F. CRISSLER

Remarks:

*Install*

*Page # 2*

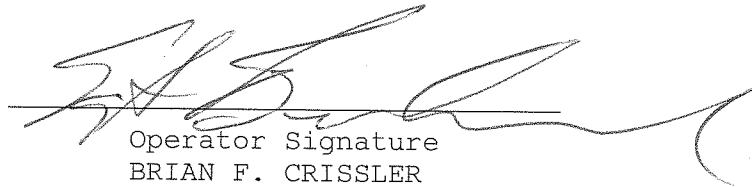
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-003067  
Location = BELC      8164.13.00 06/09  
05/06/2011      16:44

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:45
02 Std. Gas	0.080	16:45
03 Room Air	0.000	16:46
04 Std. Gas	0.079	16:46
05 Room Air	0.000	16:46
06 Std. Gas	0.080	16:47
07 Room Air	0.000	16:47

Lot No = 659357  
Cyl No = 38  
Exp Date = 09/03/2011  
County = 63      Oper No. = 119802

  
Operator Signature  
BRIAN F. CRISSLER

Remarks:

Form 106-I8000

*A/A*  
*Install page #5*

80-003067  
P. 97 of 98  
JCM

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

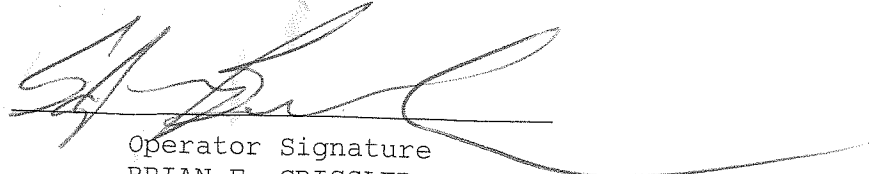
CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-003067  
Location = BELC      8164.13.00 06/09  
05/06/2011      16:41

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:42
02 Std. Gas	0.080	16:42
03 Room Air	0.000	16:43
04 Std. Gas	0.080	16:43
05 Room Air	RFI*	16:43
06 Room Air	0.000	16:44

\*Invalid Test  
Inhibited - RFI

Lot No = 659357  
Cyl No = 38  
Exp Date = 09/03/2011  
County = 63      Oper No. = 119802

  
Operator Signature  
BRIAN F. CRISSLER

Remarks:

Form 106-I8000

*Install RFI*  
*Page # 5*

80-003067  
P. 98 of 98  
1/22