



ETHANOL BREATH STANDARD CYLINDER REPORT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Sgt Brian Crissler</u>		
Location: <u>Belcourt Police Dept</u>		
Intoxilyzer® Serial Number: <u>80-003067</u>		
Gas Lot Number: <u>38 657357</u>	Gas Cylinder Number: <u>38</u>	Expiration Date: <u>9-3-2011</u>
<input checked="" type="checkbox"/> New Cylinder Installed <input type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: 0. <u>081</u> % Test 2: 0. <u>081</u> % Test 3: 0. <u>081</u> %		
(ATTACH TEST RECORD)		

Sgt Brian Crissler
Sgt Brian Crissler
 Chemical Test Operator Signature

5-6-2011
 Date

Deb Kashner
 Reviewed By

09 June 2011
 Date

Install *Page #1*

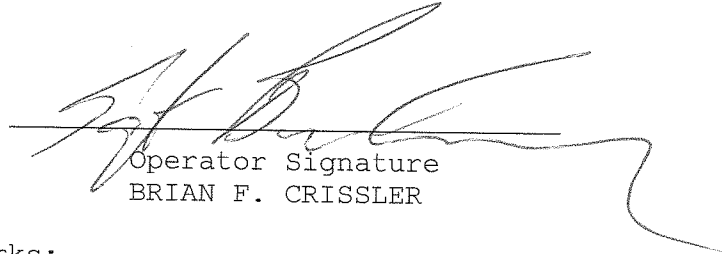
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003067
Location = BELC 8164.13.00 06/09
05/06/2011 16:37

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:37
02 Std. Gas	0.080	16:38
03 Room Air	0.000	16:38
04 Std. Gas	0.080	16:38
05 Room Air	0.000	16:39
06 Std. Gas	0.080	16:39
07 Room Air	0.000	16:40

Lot No = 659357
Cyl No = 38
Exp Date = 09/03/2011
County = 63 Oper No. = 119802


Operator Signature
BRIAN F. CRISSLER

Remarks:

Form 106-I8000

ACA
Install
page #4

80-003067
P 94 of 94
KTM