



# ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Jamie M Huschka</u>		
Location: <u>Williams Co LEC</u>		
Intoxilyzer® Serial Number: <u>80-004189</u>		
Gas Lot Number: <u>15410080A1</u>	Gas Cylinder Number: <u>6</u>	Expiration Date: <u>07/01/12</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>079</u> %		
Test 2: 0. <u>078</u> %		
Test 3: 0. <u>079</u> %		
(ATTACH TEST RECORD)		

Jamie M Huschka  
Chemical Test Operator Signature

06 May 2011  
Date

Deb Kashner  
Reviewed By

16 May 2011  
Date

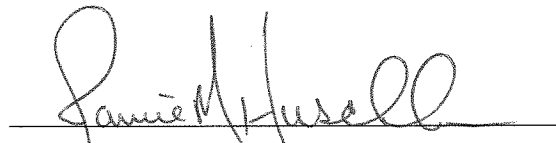
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004189  
Location = WILL      8164.13.00 06/09  
05/06/2011      19:19

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	19:20
02 Std. Gas	0.079	19:21
03 Room Air	0.000	19:21
04 Std. Gas	0.078	19:22
05 Room Air	0.000	19:22
06 Std. Gas	0.079	19:22
07 Room Air	0.000	19:23

Lot No = 15410080A1  
Cyl No = 6  
Exp Date = 07/01/2012  
County = 53      Oper No. = 100406

  
Operator Signature  
JAMIE M. HUSCHKA

Remarks:

Form 106-I8000

80-004189  
P. 132 of 132  
FM