



ETHANOL BREATH STANDARD CYLINDER REPORT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>ROBERT Kennedy</u>		
Location: <u>Rugby</u>		
Intoxilyzer® Serial Number: <u>80-004203</u>		
Gas Lot Number: <u>659358</u>	Gas Cylinder Number: <u>21</u>	Expiration Date: <u>9/3/11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: <u>0.082</u> % Test 2: <u>0.081</u> % Test 3: <u>0.081</u> %		
(ATTACH TEST RECORD)		

[Signature]
 Chemical Test Operator Signature

5/7/11
 Date

Deb Kashur
 Reviewed By

16 May 2011
 Date


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004203
Location = RUGB 8164.13.00 06/09
05/07/2011 14:09

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:10
02 Std. Gas	0.082	14:10
03 Room Air	0.000	14:11
04 Std. Gas	0.081	14:11
05 Room Air	0.000	14:12
06 Std. Gas	0.081	14:12
07 Room Air	0.000	14:13

Lot No = 659358
Cyl No = 21
Exp Date = 09/03/2011
County = 35 Oper No. = 069108

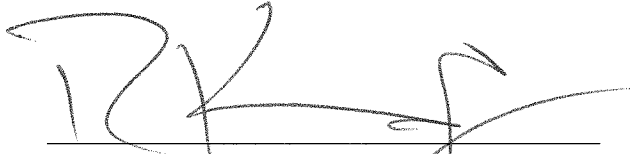

Operator Signature
ROBERT W. KENNEDY

Remarks:

Form 106-I8000

80-004203
P117 of 112
KM