

INTOXILYZER 8000 INSPECTION

Serial No.: 80-004945

Location: DKPD (DICKINSON)

- | | Check When Done |
|---|-----------------|
| A. Is the warm-up time less than 20 minutes? | <u>✓</u> |
| B. Is a three-pronged grounded outlet used? | <u>✓</u> |
| C. Is the breath tube heated? | <u>✓</u> |
| D. Is the diagnostic check complete? | <u>✓</u> |
| E. Is the time, date, and year correct (re-set if necessary)? | <u>✓</u> |
| F. Print test. (Attach test record.) | <u>✓</u> |
| G. Low AC. Use <0.03 AC in ACA mode. (Attach test record.)
Sim SN <u>DR3455</u> Lot No. <u>12210</u> Rep AC <u>0.020</u> | <u>✓</u> |
| H. Linearity Test. Use ≥ 0.25 AC in ACA mode. (Attach test record.)
Sim SN <u>DR3847</u> Lot No. <u>13020</u> Rep AC <u>0.300</u> | <u>✓</u> |
| I. Interferent check. Use 0.05% acetone plus 0.10 AC ethanol in ABA mode.
(Attach test record.)
Sim SN <u>DR5191</u> Lot No. <u>IOS#1</u> Rep AC <u>0.100AC + 0.05% ACETONE</u> | <u>✓</u> |
| J. RFI check. Run CMS mode. Key radio on first room air.
(Attach test record.) | <u>✓</u> |
| K. Calibration Check. Use Ethanol Breath Standard cylinder. Do three sets in ACA mode.
(Attach test record.) | |

Lot No. <u>23411080A1</u>	Cyl No. <u>30</u>	Exp. Date <u>10/01/2013</u>
Test 1 <u>0.081</u>	Test 4 <u>0.082</u>	Test 7 <u>0.083</u>
Test 2 <u>0.082</u>	Test 5 <u>0.082</u>	Test 8 <u>0.082</u>
Test 3 <u>0.082</u>	Test 6 <u>0.082</u>	Test 9 <u>0.083</u>
Average <u>0.082</u>		

L. Tank pressure, Level 3 Func D Sub G P: 519 psi Reg 525 psi

M. Remarks/Maintenance record: REPLACED SIMULATOR RETURN O-RING; ANNUAL INSPECTION

06 MAY 13
Date

Charles E. Ehl
Field Inspector's Signature

07 May 13
Date

Deb Kasher
Reviewed by

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = DKPD 8164.13.00 06/09
05/06/2013 16:05

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-==|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-==|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? No
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 23411080A1
Standard Cyl #? 30
Standard Expiration? 10/01/2013
Oper No? 666666

Flow Cal. Date: 09/26/2012
Slope 622
Intercept -485836

IR Calibration Date: 10/01/2012

	3um	9um
0th Coef(*100):	-23823	-20690
1st Coef(*100):	260812	140752
2nd Coef(*100):	3107	1288
H2O adj(mg/l*10k):	695	492

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks: **PRINT TEST**

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = DKPD 8164.13.00 06/09
05/06/2013 16:19

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:19
02 Std. Sol.	0.019	16:20
03 Room Air	0.000	16:20
04 Std. Sol.	0.020	16:21
05 Room Air	0.000	16:22
06 Std. Sol.	0.020	16:22
07 Room Air	0.000	16:23


08 Sim Temp = 34.0°C

Simul Ser No = DR3455

Std Sol No = 12210

County = 45

Oper No. = 666666



Operator Signature

CHARLES EDER

Remarks:

Low AC

0.020 AC (Sim. Sol.)

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = DKPD 8164.13.00 06/09
05/06/2013 16:24

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:25
02 Std. Sol.	0.302	16:26
03 Room Air	0.000	16:26
04 Std. Sol.	0.306	16:27
05 Room Air	0.000	16:27
06 Std. Sol.	0.307	16:28
07 Room Air	0.000	16:29


08 Sim Temp = 34.0°C

Simul Ser No = DR3847

Std Sol No = 13020

County = 45

Oper No. = 666666

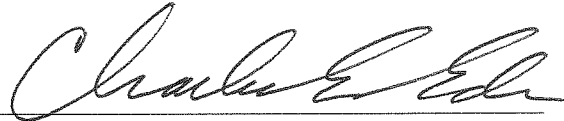

Operator Signature
CHARLES EDER

Remarks:

LINEARITY TEST
0.300 AC (SIM. SOL.)

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = DKPD 8164.13.00 06/09
05/06/2013 16:11

Test	AC	Time
01 Room Air	0.000	16:12
02 *Subject Test	INT*	16:13
03 Room Air	0.000	16:13

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = QWERTYUIOPASDFG
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 30
Expiration Date = 10/01/2013
County = 45 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *INTERFERENT CHECK*
0.100AC + 0.05% ACETONE

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = DKPD 8164.13.00 06/09
05/06/2013 16:15

Test	AC	Time
01 Diagnostic	OK	16:16
02 Room Air	RFI*	16:16
03 Room Air	0.000	16:17

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = MNBVCXZLKJH0987
Dr. Lic. = ND/DIS821456
Lot No = 23411080A1
Cyl No = 30
Expiration Date = 10/01/2013
County = 45 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = DKPD 8164.13.00 06/09
05/06/2013 16:31

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:32
02 Std. Gas	0.081	16:32
03 Room Air	0.000	16:33
04 Std. Gas	0.082	16:33
05 Room Air	0.000	16:34
06 Std. Gas	0.082	16:34
07 Room Air	0.000	16:34

Lot No = 23411080A1
Cyl No = 30
Exp Date = 10/01/2013
County = 45 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC (E.G.S.)

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = DKPD 8164.13.00 06/09
05/06/2013 16:35

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:35
02 Std. Gas	0.082	16:36
03 Room Air	0.000	16:36
04 Std. Gas	0.082	16:36
05 Room Air	0.000	16:37
06 Std. Gas	0.082	16:37
07 Room Air	0.000	16:38

Lot No = 23411080A1
Cyl No = 30
Exp Date = 10/01/2013
County = 45 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC (E.G.S.)

Form 106-I8000


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004945
Location = DKPD 8164.13.00 06/09
05/06/2013 16:38

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:39
02 Std. Gas	0.083	16:39
03 Room Air	0.000	16:39
04 Std. Gas	0.082	16:40
05 Room Air	0.000	16:40
06 Std. Gas	0.083	16:41
07 Room Air	0.000	16:41

Lot No = 23411080A1
Cyl No = 30
Exp Date = 10/01/2013
County = 45 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080AC (E.G.S.)

Form 106-I8000