



# INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59281 (5-2011)

Serial Number <b>80-004198</b>	Instrument Location <b>GFPD</b>
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

### Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. RFI Test (Use CMS Mode; Key Radio During First Room Air).
- 7. Repair and/or Maintenance Performed (if Any): \_\_\_\_\_
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>Ann Lamm</i>	Date <b>05-09-12</b>
Reviewed By (Crime Laboratory Use Only) <i>Deb Keshner</i>	Date <b>14 May 2012</b>

This record on file at the Office of Attorney General, Crime Laboratory Division, in the County of Burleigh, North Dakota, is certified to be a true and correct copy of the documents received.

Certified By: *Charles E. Edin*      Certified Date: **29 Nov. 2016**

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer  
North Dakota Model 8000 SN 80-004198  
Location = GFPD 8164.13.00 06/09  
05/09/2012 23:22

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$%^&\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$%^&\*()\_+?

Current Instrument Setup

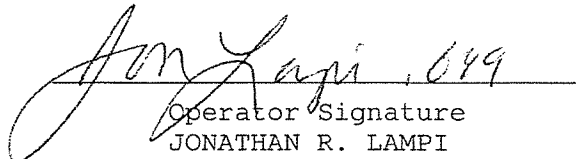
Data Entry Mode: Enabled  
Start Test Sequence: DABACABA  
Display Prelim Rslt? Yes  
Display Third Digit? Yes  
Inhib Printer(Y/N)? No  
Display Volume? No  
Disable On Memfull? Yes  
# of Print Copies? 1  
Select Std (D/W/I)? Dry  
Standard Value? 0.077  
Standard Lot #? 15410080A1  
Standard Cyl #? 37  
Standard Expiration? 07/01/2012  
Oper No? 039947

Flow Cal. Date: 01/09/2012  
Slope 637  
Intercept -467208

IR Calibration Date: 01/09/2012  
3um 9um

	3um	9um
0th Coef(*100):	-31777	-32014
1st Coef(*100):	271021	132277
2nd Coef(*100):	1454	964
H2O adj(mg/l*10k):	558	576

\*\*\*\*\* Printer Test End \*\*\*\*\*

  
Operator Signature  
JONATHAN R. LAMPI

Remarks:

Print test


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004198  
Location = GFPD      8164.13.00 06/09  
05/09/2012      23:23

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	23:24
02 Std. Gas	0.080	23:24
03 Room Air	0.000	23:25
04 Std. Gas	0.080	23:25
05 Room Air	0.000	23:26
06 Std. Gas	0.080	23:26
07 Room Air	0.000	23:26

Lot No = 15410080A1  
Cyl No = 37  
Exp Date = 07/01/2012  
County = 18      Oper No. = 039947

  
Operator Signature  
JONATHAN R. LAMPI

Remarks:

ACA test

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-004198  
Location = GFPD                    8164.13.00 06/09  
05/09/2012                            23:31

Test	AC	Time
01 Diagnostic	OK	23:32
02 Room Air	RFI*	23:32
03 Room Air	0.000	23:33

\*Invalid Test  
  Inhibited - RFI

Sub Name = CMSTEST, TEST T  
Sub DOB = 02/02/1987  
Sub Sex = Male                      Weight = 170  
Test = DUI                            Cit = 13244  
Dr. Lic. = ND/12312414  
Lot No = 15410080A1  
Cyl No = 37  
Expiration Date = 07/01/2012  
County = 18                          Oper No. = 039947

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

  
Operator Signature  
JONATHAN R. LAMPI

Remarks:

RFI TEST