



# INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59281 (03-2014)

Serial Number <b>80-006501</b>	Instrument Location <b>Grand Forks County Corrections</b>
Reason for Install/Repair <input checked="" type="checkbox"/> Install After Receiving From Crime Laboratory <input type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

### Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
  - A. Print Test (Level 1, Function P).
  - B. ACA Test (Level 1, Function C).
  - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): None
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>[Signature]</i>	Date <b>5/10/2016</b>
Reviewed By (Crime Laboratory Use Only) <i>[Signature]</i>	Date <b>16 May 2016</b>

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000            SN 80-006501  
Location = GFSO                    8164.13.00 06/09  
05/10/2016                                  21:28

\*\*\*\*\* Printer Test \*\*\*\*\*

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopQRSTUVWXYZ!@#%&^\*()\_+?

abcdefghijklmnopqrstuvwxyz1234567890- = |  
ABCDEFGHIJKLMNopQRSTUVWXYZ!@#%&^\*()\_+?

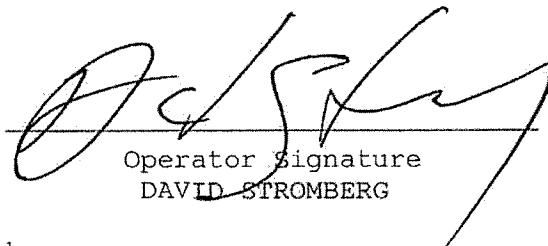
Current Instrument Setup

Data Entry Mode:            Enabled  
Start Test Sequence:        DABACABA  
Display Prelim Rslt?        Yes  
Display Third Digit?        Yes  
Inhib Printer(Y/N)?        No  
Display Volume?            No  
Disable On Memfull?        No  
# of Print Copies?         1  
Select Std (D/W/I)?        Dry  
Standard Value?            0.080  
Standard Lot #?            14214080A6  
Standard Cyl #?            52  
Standard Expiration?       07/05/2016  
Oper No?                    020836  
  
Flow Cal. Date:             08/18/2015  
Slope                        670  
Intercept                   -629984

IR Calibration Date:       08/18/2015  
                               3um                    9um

-----  
0th Coef(\*100):       -18086                    -17820  
1st Coef(\*100):       261817                   138262  
2nd Coef(\*100):       4970                      1663  
H2O adj(mg/l\*10k):    665                        427

\*\*\*\*\* Printer Test End \*\*\*\*\*

  
Operator Signature  
DAVID STROMBERG

Remarks:

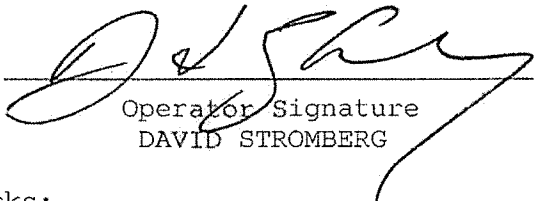
Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer            Alcohol Analyzer  
North Dakota Model 8000        SN 80-006501  
Location = GFSSO                8164.13.00 06/09  
05/10/2016                        21:29

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	21:29
02 Std. Gas	0.079	21:30
03 Room Air	0.000	21:30
04 Std. Gas	0.080	21:31
05 Room Air	0.000	21:31
06 Std. Gas	0.080	21:31
07 Room Air	0.000	21:32

Lot No = 14214080A6  
Cyl No = 52  
Exp Date = 07/05/2016  
County = 18                            Oper No. = 020836

  
Operator Signature  
DAVID STROMBERG

Remarks:

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

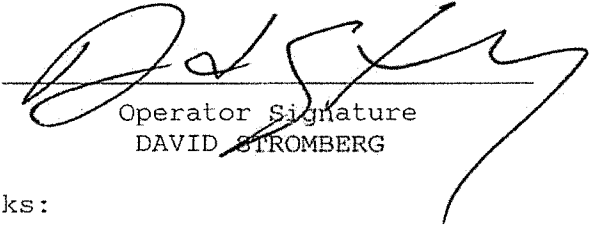
CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-006501  
Location = GFSO      8164.13.00 06/09  
05/10/2016      21:34

DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	21:34
02 Room Air	0.000	21:34

\*Invalid Test  
Inhibited - RFI

Lot No = 14214080A6  
Cyl No = 52  
Exp Date = 07/05/2016  
County = 18      Oper No. = 020836

  
Operator Signature  
DAVID STROMBERG

Remarks: