



OFFICE OF ATTORNEY GENERAL
 Crime Laboratory Division
 2641 East Main Avenue
 P.O. Box 937
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

ETHANOL BREATH STANDARD CYLINDER INSTALLATION FORM

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Richard D. Johnson

Location: McLean S.O., Washburn ND

Intoxilyzer Serial No.: 80-004196

Lot Number: ¹⁵~~47~~ 659357

Cylinder Number: 47

Expiration Date: 9/3/11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 081 %

Test 2: 0. 081 %

Test 3: 0. 080 %

(ATTACH TEST RECORD)

Richard D. Johnson
 Chemical Test Operator Signature

5/12/2010
 Date Cylinder Changed

Deb Kasher
 Reviewed By

17 May 2010
 Date

Form 105-G
 Toxicology Laboratory
 Crime Laboratory Division

80-004196
 P. 78/79 KSM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004196
Location = WASH 8164.13.00 06/09
05/12/2010 10:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:17
02 Std. Gas	0.081	10:17
03 Room Air	0.000	10:18
04 Std. Gas	0.081	10:18
05 Room Air	0.000	10:19
06 Std. Gas	0.080	10:19
07 Room Air	0.000	10:20

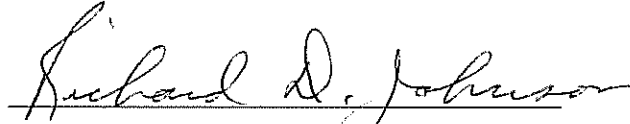
Lot No = 659357

Cyl No = 47

Exp Date = 09/03/2011

County = 28

Oper No. = 118707


Operator Signature
RICHARD D. JOHNSON

Remarks:

Form 106-I8000

80-004196
P. 79/99 SEM