



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION

Toxicology Section/Breath Alcohol Program

SFN 59282 (5-2011)

Chemical Test Operator Name (Print) <i>GARY SANDERS</i>		
Location <i>Linton ND</i>	Intoxilyzer® Serial Number <i>80-004946</i>	
Gas Lot Number <i>23411080A1</i>	Gas Cylinder Number <i>09</i>	Gas Expiration Date <i>10-1-2013</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 - A. *0.081* AC
 - B. *0.080* AC
 - C. *0.080* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Breath Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature <i>Gary Sanders</i>	Date <i>5-18-12</i>
Reviewed By (Crime Laboratory Use Only) <i>Deb Kashner</i>	Date <i>18 May 12</i>

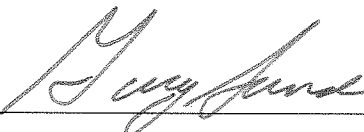
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004946
Location = LINT 8164.13.00 06/09
05/18/2012 09:31

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	09:32
02 Std. Gas	0.081	09:32
03 Room Air	0.000	09:33
04 Std. Gas	0.080	09:33
05 Room Air	0.000	09:33
06 Std. Gas	0.080	09:34
07 Room Air	0.000	09:34

Lot No = 23411080A1
Cyl No = 9
Exp Date = 10/01/2013
County = 15 Oper No. = 099418


Operator Signature
GARY R. SANDERS

Remarks: