

INTOXILYZER 8000 INSPECTION

Serial No.: 80-4206⁰⁰⁴²⁰⁶

Location: TOXL

- | | Check When Done |
|---|-----------------|
| A. Is the warm-up time less than 20 minutes? | <u>✓</u> |
| B. Is a three-pronged grounded outlet used? | <u>✓</u> |
| C. Is the breath tube heated? | <u>✓</u> |
| D. Is the diagnostic check complete? | <u>✓</u> |
| E. Is the time, date, and year correct (re-set if necessary)? | <u>✓</u> |
| F. Print test. (Attach test record.) | <u>✓</u> |
| G. Low AC. Use <0.03 AC in ACA mode. (Attach test record.)
Sim SN <u>DR5144</u> Lot No. <u> </u> Rep AC <u>0.021</u> | <u>✓</u> |
| H. Linearity Test. Use ≥ 0.25 AC in ACA mode. (Attach test record.)
Sim SN <u>DR3847</u> Lot No. <u> </u> Rep AC <u>0.294</u> | <u>✓</u> |
| I. Interferent check. Use 0.05% acetone plus 0.10 AC ethanol in ABA mode.
(Attach test record.)
Sim SN <u>DR3452</u> Lot No. <u> </u> Rep AC <u>0.10AC + Acetone</u> | <u>✓</u> |
| J. RFI check. Run CMS mode. Key radio on first room air.
(Attach test record.) | <u>✓</u> |
| K. Calibration Check. Use Ethanol Breath Standard cylinder. Do three sets in ACA mode.
(Attach test record.) | |

Lot No. <u>15410080A1</u>	Cyl No. <u>21</u>	Exp. Date <u>7-1-12</u>
Test 1 <u>0.080</u>	Test 4 <u>0.080</u>	Test 7 <u>0.080</u>
Test 2 <u>0.080</u>	Test 5 <u>0.080</u>	Test 8 <u>0.079</u>
Test 3 <u>0.080</u>	Test 6 <u>0.079</u>	Test 9 <u>0.080</u>
Average <u>0.080</u>		

L. Tank pressure, Level 3 Func D Sub G P: 172 psi Reg 180 psi

M. Remarks/Maintenance record: Annual Insp Inspection
5-19-11 Date 19 May 2011
Field Inspector's Signature Deb Kashner
Reviewed by

80-004206
p. 121 of 129
km

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004206
Location = TOXL 8164.13.00 06/09
05/19/2011 10:32

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNPOQRSTUVWXYZ!@#\$\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer (Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 15410080A1
Standard Cyl #? 21
Standard Expiration? 07/01/2012
Oper No? 555555

Flow Cal. Date: 06/10/2009
Slope 690
Intercept -645883

IR Calibration Date: 06/07/2010
 3um 9um

0th Coef(*100): -17579 -21810
1st Coef(*100): 254057 127149
2nd Coef(*100): 4591 1650
H2O adj(mg/l*10k): 756 795

***** Printer Test End *****



Operator Signature
ASHLEY AYD

Remarks: *Print test*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004206
Location = TOXL 8164.13.00 06/09
05/19/2011 10:46

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:47
02 Std. Sol.	0.019	10:48
03 Room Air	0.000	10:49
04 Std. Sol.	0.019	10:49
05 Room Air	0.000	10:50
06 Std. Sol.	0.019	10:50
07 Room Air	0.000	10:51


08 Sim Temp = 34.0°C

Simul Ser No = 0

Std Sol No = 0

County = 08

Oper No. = 555555

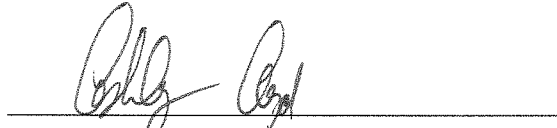

Operator Signature
ASHLEY AYD

Remarks: *Low AC 0.021AC*

Form 106-I8000

*80-004206
p. 123 of 129
YAM*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004206
Location = TOXL 8164.13.00 06/09
05/19/2011 10:52

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:52
02 Std. Sol.	0.295	10:53
03 Room Air	0.000	10:54
04 Std. Sol.	0.296	10:54
05 Room Air	0.000	10:55
06 Std. Sol.	0.296	10:56
07 Room Air	0.000	10:56

08 Sim Temp = 34.0°C

Simul Ser No = 0
Std Sol No = 0
County = 08 Oper No. = 555555



Operator Signature
ASHLEY AYD

Remarks: *Linearity test 0.294AC*

Form 106-I8000

80-004206
p.124 of 129
KM


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004206
Location = TOXL 8164.13.00 06/09
05/19/2011 10:42

Test	AC	Time
01 Room Air	0.000	10:43
02 *Subject Test	INT*	10:43
03 Room Air	0.000	10:44

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 15410080A1
Cyl No = 21
Expiration Date = 07/01/2012
County = 08 Oper No. = 555555



Operator Signature
ASHLEY AYD

Remarks: *Interferent check 0.10AC+Acetone*

Form 106-I8000

80-004206
P. 125 of 129
SM

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004206
Location = TOXL 8164.13.00 06/09
05/19/2011 10:44

Test	AC	Time
01 Diagnostic	OK	10:45
02 Room Air	RFI*	10:45
03 Room Air	0.000	10:46

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = NA
Dr. Lic. = ND/DIS821456
Lot No = 15410080A1
Cyl No = 21
Expiration Date = 07/01/2012
County = 08 Oper No. = 555555

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
ASHLEY AYD

Remarks: RFI

Form 106-I8000

80-004206
P. 126 of 129
JFM


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004206
Location = TOXL 8164.13.00 06/09
05/19/2011 10:32

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:32
02 Std. Gas	0.080	10:33
03 Room Air	0.000	10:33
04 Std. Gas	0.080	10:34
05 Room Air	0.000	10:34
06 Std. Gas	0.080	10:35
07 Room Air	0.000	10:35

Lot No = 15410080A1
Cyl No = 21
Exp Date = 07/01/2012
County = 08 Oper No. = 555555

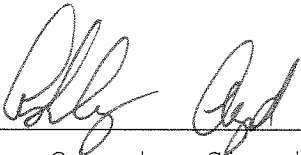

Operator Signature
ASHLEY AYD

Remarks: *Calibration check 0.080 AC*

Form 106-I8000

*80-004206
P127 of 129
JTM*


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004206
Location = TOXL 8164.13.00 06/09
05/19/2011 10:35

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:36
02 Std. Gas	0.080	10:36
03 Room Air	0.000	10:37
04 Std. Gas	0.080	10:37
05 Room Air	0.000	10:38
06 Std. Gas	0.079	10:38
07 Room Air	0.000	10:38

Lot No = 15410080A1
Cyl No = 21
Exp Date = 07/01/2012
County = 08 Oper No. = 555555



Operator Signature
ASHLEY AYD

Remarks: Calibration check 0.080 AC

Form 106-I8000

80-004206
P. 128 of 129
KAM


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004206
Location = TOXL 8164.13.00 06/09
05/19/2011 10:39

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:39
02 Std. Gas	0.080	10:40
03 Room Air	0.000	10:40
04 Std. Gas	0.079	10:40
05 Room Air	0.000	10:41
06 Std. Gas	0.080	10:41
07 Room Air	0.000	10:42

Lot No = 15410080A1
Cyl No = 21
Exp Date = 07/01/2012
County = 08 Oper No. = 555555



Operator Signature
ASHLEY AYD

Remarks: Calibration check 0.080AC

Form 106-I8000

80-004206
P.129 of 129
JTM