

INTOXILYZER® 8000 INSPECTION

Serial No.: 80-005939

Location: CASS

- | | Check When Done |
|---|-----------------|
| A. Is the breath tube heated? | <u>✓</u> |
| B. Is the diagnostic check complete? | <u>✓</u> |
| C. Is the time, date, and year correct (re-set if necessary)? | <u>✓</u> |
| D. Print test. (Attach test record.) | <u>✓</u> |
| E. Low AC. Use <0.03 AC in ACA mode. (Attach test record.)
Sim SN <u>DR5115</u> Lot No. <u>12111</u> Rep AC <u>0.020</u> | <u>✓</u> |
| F. High AC. Use ≥ 0.25 AC in ACA mode. (Attach test record.)
Sim SN <u>DR5143</u> Lot No. <u>13080</u> Rep AC <u>0.300</u> | <u>✓</u> |
| G. Interferent check. Use 0.05% acetone plus 0.10 AC ethanol in ABA mode.
(Attach test record.)
Sim SN <u>DR3375</u> Lot No. <u>ICS#2</u> Rep AC <u>0.100AC + 0.05% ACETONE</u> | <u>✓</u> |
| H. RFI check. Run CMS mode. Key radio on first room air.
(Attach test record.) | <u>✓</u> |
| I. Calibration Check. Use Ethanol Breath Standard cylinder. Do three sets in ACA mode.
(Attach test record.) | |

Lot No. 16512080A2 Cyl No. 066 Exp. Date 08/01/2014

Test 1 <u>0.082</u>	Test 4 <u>0.083</u>	Test 7 <u>0.083</u>
Test 2 <u>0.082</u>	Test 5 <u>0.083</u>	Test 8 <u>0.083</u>
Test 3 <u>0.082</u>	Test 6 <u>0.082</u>	Test 9 <u>0.082</u>

Average 0.082

J. Tank pressure, Level 3 Func D Sub G P: 148 psi Reg 150 psi

K. Remarks/Maintenance record: ANNUAL INSPECTION

14 MAY 14
Date

19 May 14 ✓
Date

Charles E. Eden
Field Inspector's Signature

Deb Kasher
Reviewed by

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = CASS 8164.13.00 06/09
05/14/2014 17:47

***** Printer Test *****

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

abcdefghijklmnopqrstuvwxy1234567890-=
ABCDEFGHIJKLMNopqrstuvwxyz!@#%&^*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 16512080A2
Standard Cyl #? 66
Standard Expiration? 08/01/2014
Oper No? 666666

Flow Cal. Date: 06/18/2013
Slope 676
Intercept -672473

IR Calibration Date: 06/18/2013

	3um	9um
0th Coef(*100):	-16377	-17793
1st Coef(*100):	286199	137970
2nd Coef(*100):	3159	1297
H2O adj(mg/l*10k):	522	398

***** Printer Test End *****



Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = CASS 8164.13.00 06/09
05/14/2014 17:50

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	17:51
02 Std. Sol.	0.019	17:52
03 Room Air	0.000	17:52
04 Std. Sol.	0.019	17:53
05 Room Air	0.000	17:53
06 Std. Sol.	0.020	17:54
07 Room Air	0.000	17:55

08 Sim Temp = 34.0°C

Simul Ser No = DR5115
Std Sol No = 12111
County = 09 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *Low AC*
0.020 AC

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = CASS 8164.13.00 06/09
05/14/2014 17:57

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	17:57
02 Std. Sol.	0.290	17:58
03 Room Air	0.000	17:59
04 Std. Sol.	0.293	17:59
05 Room Air	0.000	18:00
06 Std. Sol.	0.294	18:01
07 Room Air	0.000	18:01

08 Sim Temp = 34.0°C

Simul Ser No = DR5143
Std Sol No = 13080
County = 09 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *HIGH AC*
0.300 AC

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = CASS 8164.13.00 06/09
05/14/2014 18:03

Test	AC	Time
01 Room Air	0.000	18:04
02 *Subject Test	INT*	18:05
03 Room Air	0.000	18:05

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 16512080A2
Cyl No = 66
Expiration Date = 08/01/2014
County = 09 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: *INTERFERENT CHECK*
0.100AC + 0.05% ACETONE

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = CASS 8164.13.00 06/09
05/14/2014 18:05

Test	AC	Time
01 Diagnostic	OK	18:06
02 Room Air	RFI*	18:07
03 Room Air	0.000	18:07

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS821456
Lot No = 16512080A2
Cyl No = 66
Expiration Date = 08/01/2014
County = 09 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.

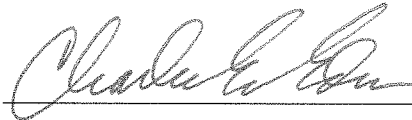

Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = CASS 8164.13.00 06/09
05/14/2014 18:08

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:08
02 Std. Gas	0.082	18:09
03 Room Air	0.000	18:09
04 Std. Gas	0.082	18:09
05 Room Air	0.000	18:10
06 Std. Gas	0.082	18:10
07 Room Air	0.000	18:11

Lot No = 16512080A2
Cyl No = 66
Exp Date = 08/01/2014
County = 09 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = CASS 8164.13.00 06/09
05/14/2014 18:11

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:12
02 Std. Gas	0.083	18:12
03 Room Air	0.000	18:13
04 Std. Gas	0.083	18:13
05 Room Air	0.000	18:14
06 Std. Gas	0.082	18:14
07 Room Air	0.000	18:14

Lot No = 16512080A2
Cyl No = 66
Exp Date = 08/01/2014
County = 09 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION ^{CBE} ~~CHECK~~ CHECK
0.080 AC


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005939
Location = CASS 8164.13.00 06/09
05/14/2014 18:15

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:15
02 Std. Gas	0.083	18:15
03 Room Air	0.000	18:16
04 Std. Gas	0.083	18:16
05 Room Air	0.000	18:17
06 Std. Gas	0.082	18:17
07 Room Air	0.000	18:18

Lot No = 16512080A2
Cyl No = 66
Exp Date = 08/01/2014
County = 09 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC