



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name:	Duane L. Marmor				
Location:	STAN				
Intoxilyzer® Serial Number:	80-004943				
Gas Lot Number:	709352	Gas Cylinder Number:	34	Expiration Date:	12/23/2011
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed				
Instrument Test Results (Report to 3 Digits; Example, 0.081%)					
Test 1: 0.079%					
Test 2: 0.079%					
Test 3: 0.079%					
(ATTACH TEST RECORD)					



Chemical Test Operator Signature

05/24/10

Date

Deb Kashner

Reviewed By

27 May 2010

Date


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004943
Location = STAN 8164.13.00 06/09
05/24/2010 20:39

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	20:39
02 Std. Gas	0.079	20:40
03 Room Air	0.000	20:40
04 Std. Gas	0.079	20:40
05 Room Air	0.000	20:41
06 Std. Gas	0.079	20:41
07 Room Air	0.000	20:42

Lot No = 709352
Cyl No = 34
Exp Date = 12/23/2011
County = 31 Oper No. = 100019

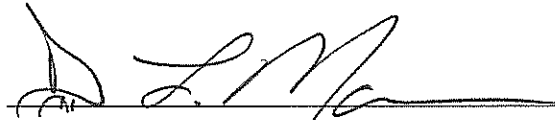

Operator Signature
DUANE L. MARMON

Remarks:

Form 106-I8000

80-004943
P. 42/42 FM