



OFFICE OF ATTORNEY GENERAL  
 Crime Laboratory Division  
 2641 East Main Avenue  
 P.O. Box 937  
 Bismarck, North Dakota 58502-0937

TEL 701-328-6159

**ETHANOL BREATH STANDARD CYLINDER INSTALLATION FORM**

(Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.)

Chemical Test Operator Name: Pete Nielsen

Location: West Fargo PD

Intoxilyzer Serial No.: 80-063059

Lot Number: 659357

Cylinder Number: 10

Expiration Date: 9-3-11

Instrument Test Results (Report to 3 Digits; Example, 0.081%)

Test 1: 0. 080 %

Test 2: 0. 080 %

Test 3: 0. 080 %

(ATTACH TEST RECORD)

[Signature]  
 Chemical Test Operator Signature

5-25-10  
 Date Cylinder Changed

Deb Kashur

27 May 2010

Form 105-G  
 Toxicology Laboratory  
 Crime Laboratory Division

80-003059  
 P. 82/83 FM


Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-003059  
Location = WFPD      8164.13.00 06/09  
05/25/2010      14:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:49
02 Std. Gas	0.080	14:49
03 Room Air	0.000	14:50
04 Std. Gas	0.080	14:50
05 Room Air	0.000	14:51
06 Std. Gas	0.080	14:51
07 Room Air	0.000	14:52

Lot No = 659357  
Cyl No = 10  
Exp Date = 09/03/2011  
County = 09      Oper No. = 039617

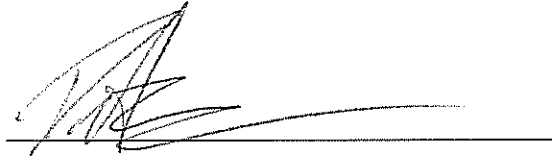

Operator Signature  
PETER NIELSEN

Remarks:

Form 106-I8000

80-003059  
P. 83/83 JAL