

INTOXILYZER® 8000 INSPECTION

Serial No.: 80-003072

Location: GARR ^{GARRISON}
_(McLEAN COUNTY, S.D.)

- | | Check When Done |
|--|-----------------|
| A. Is the breath tube heated? | <u>✓</u> |
| B. Is the diagnostic check complete? | <u>✓</u> |
| C. Is the time, date, and year correct (re-set if necessary)? | <u>✓</u> |
| D. Print test. (Attach test record.) | <u>✓</u> |
| E. Low AC. Use ≤ 0.03 AC in ACA mode. (Attach test record.)
Sim SN <u>DR5191</u> Lot No. <u>15160</u> Rep AC <u>0.020</u> | <u>✓</u> |
| F. High AC. Use ≥ 0.25 AC in ACA mode. (Attach test record.)
Sim SN <u>DR3847</u> Lot No. <u>16060</u> Rep AC <u>0.300</u> | <u>✓</u> |
| G. Interferent check. Use 0.05% acetone in ethanol solution in ABA mode.
(Attach test record.)
Sim SN <u>DR5190</u> Lot No. <u>ICS4</u> Solution <u>0.10AC + 0.05% ACETONE</u> | <u>✓</u> |
| H. RFI check. Run CMS mode. Key radio during CMS test.
(Attach test record.) | <u>✓</u> |

I. Calibration Check. Use Ethanol Breath Standard cylinder. Do three sets in ACA mode.
(Attach test record.) 0.080 AC

Lot No. 29614080A2 Cyl No. 33 Exp. Date 12/05/2016

Test 1 <u>0.081</u>	Test 4 <u>0.082</u>	Test 7 <u>0.081</u>
Test 2 <u>0.081</u>	Test 5 <u>0.081</u>	Test 8 <u>0.081</u>
Test 3 <u>0.082</u>	Test 6 <u>0.081</u>	Test 9 <u>0.081</u>

Average 0.081

J. Tank pressure, Level 3 Func D Sub G P: 1016 psi Reg ~1000 psi

K. Remarks/Maintenance record: ANNUAL INSPECTION

5/26/2016
Date
27
DS-28 May 2016
Date

Charles E. Ed
Field Inspector's Signature
Deb Shanaver
Reviewed by

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = GARR 8164.13.00 06/09
05/26/2016 14:46

***** Printer Test *****

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

abcdefghijklmnopqrstuvwxyz1234567890-=_|
ABCDEFGHIJKLMNopqrstuvwxyz!@#\$\$%^&*()_+?

Current Instrument Setup


Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On Memfull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #? 29614080A2
Standard Cyl #? 33
Standard Expiration? 12/05/2016
Oper No? 666666

Flow Cal. Date: 03/09/2011
Slope 682
Intercept -620512

IR Calibration Date: 03/09/2011
 3um 9um

	3um	9um
0th Coef(*100):	-24766	-17499
1st Coef(*100):	264559	138630
2nd Coef(*100):	1876	1114
H2O adj(mg/l*10k):	497	331

***** Printer Test End *****

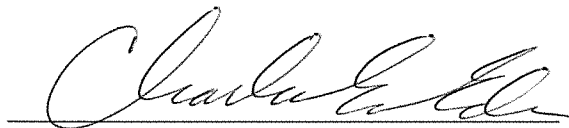

Operator Signature
CHARLES EDER

Remarks:

PRINT TEST

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = GARR 8164.13.00 06/09
05/26/2016 15:08

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:08
02 Std. Sol.	0.017	15:09
03 Room Air	0.000	15:10
04 Std. Sol.	0.017	15:10
05 Room Air	0.000	15:11
06 Std. Sol.	0.018	15:12
07 Room Air	0.000	15:12

08 Sim Temp = 34.0°C

Simul Ser No = DR5191
Std Sol No = 15160
County = 28 Oper No. = 666666

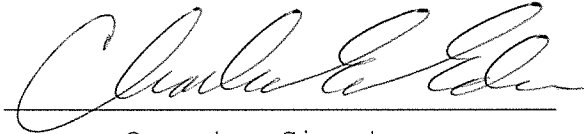

Operator Signature
CHARLES EDER

Remarks:

Low AC
0.020 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = GARR 8164.13.00 06/09
05/26/2016 15:14

WET CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:15
02 Std. Sol.	0.296	15:16
03 Room Air	0.000	15:16
04 Std. Sol.	0.302	15:17
05 Room Air	0.000	15:17
06 Std. Sol.	0.304	15:18
07 Room Air	0.000	15:19


08 Sim Temp = 34.0°C

Simul Ser No = DR3847

Std Sol No = 16060

County = 28

Oper No. = 666666

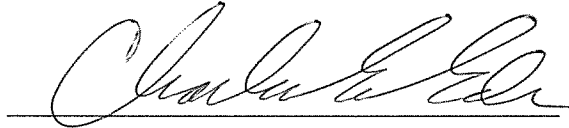

Operator Signature
CHARLES EDER

Remarks:

HIGH AC
0.300 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = GARR 8164.13.00 06/09
05/26/2016 14:59

Test	AC	Time
01 Room Air	0.000	15:00
02 *Subject Test	INT*	15:01
03 Room Air	0.000	15:02

*Invalid Test
Interferent Detected

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = INTERFERENT
Dr. Lic. = ND/DIS821456
Lot No = 29614080A2
Cyl No = 33
Expiration Date = 12/05/2016
County = 28 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks:

Interferent Check
0.10Ac + 0.05% ACETONE

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501


CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = GARR 8164.13.00 06/09
05/26/2016 15:03

Test	AC	Time
01 Diagnostic	OK	15:04
02 Room Air	0.000	15:05
03 *Subject Test	RFI*	15:05
04 Room Air	0.000	15:05

*Invalid Test
Inhibited - RFI

Sub Name = DISCOVER, THE SPIRIT
Sub DOB = 01/01/1982
Sub Sex = Female Weight = 150
Test = DUI Cit = RFI CHECK
Dr. Lic. = ND/DIS821456
Lot No = 29614080A2
Cyl No = 33
Expiration Date = 12/05/2016
County = 28 Oper No. = 666666

I followed the Approved Method and the instructions displayed by the Intoxilyzer in conducting this test.



Operator Signature
CHARLES EDER

Remarks: *RFI CHECK*


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = GARR 8164.13.00 06/09
05/26/2016 15:22

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:22
02 Std. Gas	0.081	15:23
03 Room Air	0.000	15:23
04 Std. Gas	0.081	15:23
05 Room Air	0.000	15:24
06 Std. Gas	0.082	15:24
07 Room Air	0.000	15:25

Lot No = 29614080A2
Cyl No = 33
Exp Date = 12/05/2016
County = 28 Oper No. = 666666

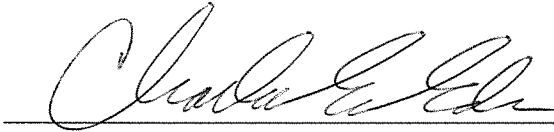

Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = GARR 8164.13.00 06/09
05/26/2016 15:25

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:26
02 Std. Gas	0.082	15:26
03 Room Air	0.000	15:27
04 Std. Gas	0.081	15:27
05 Room Air	0.000	15:27
06 Std. Gas	0.081	15:28
07 Room Air	0.000	15:28

Lot No = 29614080A2
Cyl No = 33
Exp Date = 12/05/2016
County = 28 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK

0.080 AC

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003072
Location = GARR 8164.13.00 06/09
05/26/2016 15:29

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:29
02 Std. Gas	0.081	15:30
03 Room Air	0.000	15:30
04 Std. Gas	0.081	15:31
05 Room Air	0.000	15:31
06 Std. Gas	0.081	15:32
07 Room Air	0.000	15:32

Lot No = 29614080A2
Cyl No = 33
Exp Date = 12/05/2016
County = 28 Oper No. = 666666



Operator Signature
CHARLES EDER

Remarks: CALIBRATION CHECK
0.080 AC

Form 106-I8000