



ETHANOL GAS STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (10-2013)

Chemical Test Operator Name (Print) ROBERT KENNEDY		
Location DEVILS LAKE LEC	Intoxilyzer® Serial Number 80-005954	
Gas Lot Number 09216080A3	Gas Cylinder Number 25	Gas Expiration Date 5/5/2018

Check When Done:

1. Scan/Enter Gas Cylinder Information (Level 1, Function S).

2. Perform an ACA Test (Level 1, Function C).

Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).

A. 0.080 AC

B. 0.080 AC

C. 0.080 AC

3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.

4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.

5. Send the Following to the Crime Laboratory:

A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).

B. ACA Test Record.

Chemical Test Operator Signature [Signature] #277NDAP	Date 5/29/2016 ✓
Reviewed By (Crime Laboratory Use Only) Deb Shaver	Date 02 June 16


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005954
Location = DEVL 8164.13.00 06/09
05/29/2016 14:07

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:07
02 Std. Gas	0.080	14:08
03 Room Air	0.000	14:08
04 Std. Gas	0.080	14:09
05 Room Air	0.000	14:09
06 Std. Gas	0.080	14:10
07 Room Air	0.000	14:10

Lot No = 09216080A3
Cyl No = 25
Exp Date = 05/05/2018
County = 36 Oper No. = 069108

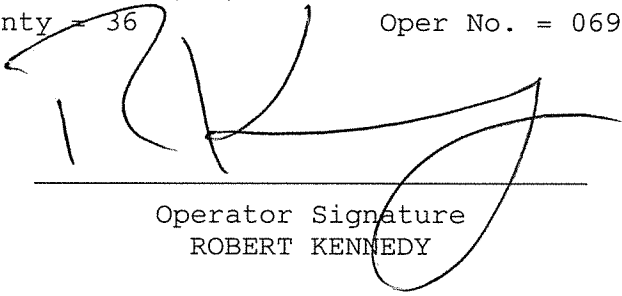

Operator Signature
ROBERT KENNEDY

Remarks: