



ETHANOL BREATH STANDARD CYLINDER REPORT
OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <i>Lt. Tracy L. Meidinger #258</i>		
Location: <i>UNO-PD</i>		
Intoxilyzer® Serial Number: <i>80-004934</i>		
Gas Lot Number: <i>659358</i>	Gas Cylinder Number: <i>31</i>	Expiration Date: <i>09-03-2011</i>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u><i>079</i></u> %		
Test 2: 0. <u><i>080</i></u> %		
Test 3: 0. <u><i>080</i></u> %		
(ATTACH TEST RECORD)		

Lt. Tracy L. Meidinger

Chemical Test Operator Signature

06-01-10

Date

Deb Kashur

Reviewed By

03 June 2010

Date

80-004934
P. 48 of 49
KRM

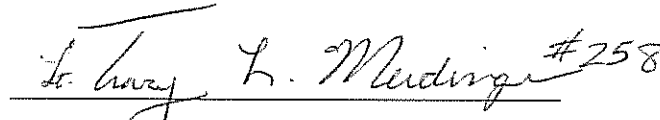
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004934
Location = UNDP 8164.13.00 06/09
06/01/2010 19:20

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	19:21
02 Std. Gas	0.079	19:21
03 Room Air	0.000	19:22
04 Std. Gas	0.080	19:22
05 Room Air	0.000	19:23
06 Std. Gas	0.080	19:23
07 Room Air	0.000	19:24

Lot No = 659358
Cyl No = 31
Exp Date = 09/03/2011
County = 18 Oper No. = 119409


Operator Signature
TRACY L. MEIDINGER

Remarks:

Form 106-I8000

ACA June 2010

80-004934
P. 49 of 49
YAM