



ETHANOL GAS STANDARD CYLINDER REPORT
 OFFICE OF ATTORNEY GENERAL
 CRIME LABORATORY DIVISION
 Toxicology Section/Breath Alcohol Program
 SFN 59282 (10-2013)

Chemical Test Operator Name (Print) <u>KEVIN A. HUSTON</u>		
Location <u>WARD COUNTY JAIL</u>	Intoxilyzer® Serial Number <u>80-004193</u>	
Gas Lot Number <u>09216080A3</u>	Gas Cylinder Number <u>32</u>	Gas Expiration Date <u>5-5-18</u>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
 Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 A. 0.080 AC
 B. 0.079 AC
 C. 0.079 AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Gas Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature <u>[Signature]</u>	Date <u>6-30-16</u>
Reviewed By (Crime Laboratory Use Only) <u>Deb Shanaver</u>	Date <u>30 June 16</u>

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004193
Location = WARD 8164.13.00 06/09
06/30/2016 10:57

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	10:57
02 Std. Gas	0.080	10:58
03 Room Air	0.000	10:58
04 Std. Gas	0.079	10:59
05 Room Air	0.000	10:59
06 Std. Gas	0.079	10:59
07 Room Air	0.000	11:00


Lot No = 09216080A3

Cyl No = 32

Exp Date = 05/05/2018

County = 51

Oper No. = 039709

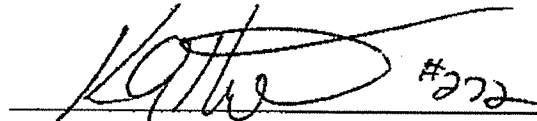

Operator Signature
KEVIN HUSTON

Remarks:

Form 106-I8000