



ETHANOL BREATH STANDARD CYLINDER REPORT
OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Jonathan Tofteland</u>		
Location: <u>MohL</u>		
Intoxilyzer® Serial Number: <u>80-004198</u>		
Gas Lot Number: <u>659358</u>	Gas Cylinder Number: <u>27</u>	Expiration Date: <u>9-3-11</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.076</u> %		
Test 2: <u>0.070</u> %		
Test 3: <u>0.077</u> %		
(ATTACH TEST RECORD)		

[Signature]
Chemical Test Operator Signature

7-1-10
Date

Deb Kashner
Reviewed By

06 July 2010
Date

80-004198
P. 95 of 96
KH


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = MOHL 8164.13.00 06/09
07/01/2010 16:43

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	16:43
02 Std. Gas	0.076	16:44
03 Room Air	0.000	16:44
04 Std. Gas	0.076	16:44
05 Room Air	0.000	16:45
06 Std. Gas	0.077	16:45
07 Room Air	0.000	16:46

Lot No = 659358
Cyl No = 27
Exp Date = 09/03/2011
County = 38 Oper No. = 100915

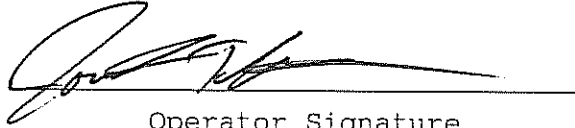

Operator Signature
JONATHAN M. TOFTELAND

Remarks:

Form 106-I8000

80-004198
P. 9/6/09
JMT