



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL

CRIME LABORATORY DIVISION

Toxicology Section/Breath Alcohol Program

SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Dean Hoaland</u>		
Location: <u>Cass Jail</u>		
Intoxilyzer® Serial Number: <u>80-004205</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>14</u>	Expiration Date: <u>12-23-2011</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: <u>0.080</u> %		
Test 2: <u>0.080</u> %		
Test 3: <u>0.080</u> %		
(ATTACH TEST RECORD)		

Dean Hoaland
Chemical Test Operator Signature

7-7-10
Date

Deb Kashur
Reviewed By

13 July 2010
Date

80-004205^{SFN}
8/8/10 AKL


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004205
Location = CASS 8164.13.00 06/09
07/01/2010 15:13

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	15:13
02 Std. Gas	0.080	15:14
03 Room Air	0.000	15:14
04 Std. Gas	0.080	15:15
05 Room Air	0.000	15:15
06 Std. Gas	0.080	15:16
07 Room Air	0.000	15:16

Lot No = 709352
Cyl No = 14
Exp Date = 12/23/2011
County = 09 Oper No. = 109409

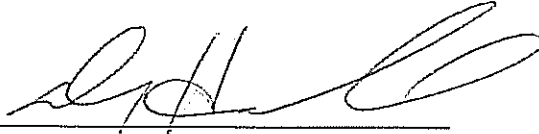

Operator Signature
DEAN J. HAALAND

Remarks:

Form 106-I8000

80-004205
8/8/09 KM