



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Lori Flaten</u>		
Location: <u>MAND</u>		
Intoxilyzer® Serial Number: <u>80-004939</u>		
Gas Lot Number: <u>659358</u>	Gas Cylinder Number: <u>40</u>	Expiration Date: <u>09-03-11</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>079</u> %		
Test 2: 0. <u>079</u> %		
Test 3: 0. <u>079</u> %		
(ATTACH TEST RECORD)		

[Signature]
Chemical Test Operator Signature

07-01-10
Date

Deb Kasher
Reviewed By

07 July 2010
Date


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004939
Location = TOXL 8164.13.00 06/09
07/01/2010 14:48

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	14:49
02 Std. Gas	0.079	14:49
03 Room Air	0.000	14:49
04 Std. Gas	0.079	14:50
05 Room Air	0.000	14:50
06 Std. Gas	0.079	14:51
07 Room Air	0.000	14:51

Lot No = 659358
Cyl No = 40
Exp Date = 09/03/2011
County = 30 Oper No. = 068019

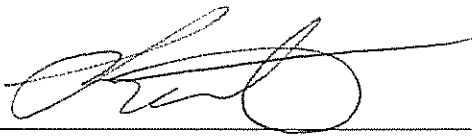

Operator Signature
LORI E. FLATEN

Remarks:

Form 106-I8000

80-004939
P. 38 of 38 PM