



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>David M Wallace</u>		
Location: <u>Dickinson</u>		
Intoxilyzer® Serial Number: <u>80-004947</u>		
Gas Lot Number: <u>659358</u>	Gas Cylinder Number: <u>23</u>	Expiration Date: <u>9-3-11</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
<p>Instrument Test Results (Report to 3 Digits; Example, 0.081%)</p> <p>Test 1: 0. <u>077</u> %</p> <p>Test 2: 0. <u>078</u> %</p> <p>Test 3: 0. <u>078</u> %</p> <p style="text-align: right;">(ATTACH TEST RECORD)</p>		

David M Wallace
Chemical Test Operator Signature

7-2-10
Date

Deb Kashner
Reviewed By

08 July 2010
Date

80-004947
P. 45446
JW

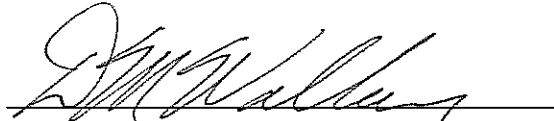
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004947
Location = DKPD 8164.13.00 06/09
07/02/2010 07:57

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	07:58
02 Std. Gas	0.077	07:58
03 Room Air	0.000	07:58
04 Std. Gas	0.078	07:59
05 Room Air	0.000	07:59
06 Std. Gas	0.078	08:00
07 Room Air	0.000	08:00

Lot No = 659358
Cyl No = 23
Exp Date = 09/03/2011
County = 45 Oper No. = 068332


Operator Signature
DAVID M. WALLACE

Remarks:

Form 106-I8000

80-004947
P. 46 of 46
JAW