



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Aaron Hummel</u>		
Location: <u>GFSO</u>		
Intoxilyzer® Serial Number: <u>80-003057</u>		
Gas Lot Number: <u>659357</u>	Gas Cylinder Number: <u>26</u>	Expiration Date: <u>9/3/11</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>080</u> %		
Test 2: 0. <u>080</u> %		
Test 3: 0. <u>080</u> %		
(ATTACH TEST RECORD)		

Aaron Hummel
Chemical Test Operator Signature

7/26/10
Date

Deb Kashur
Reviewed By

03 Aug 2010
Date

80-003057
P. 103 of 104
KH


Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-003057
Location = GFSO 8164.13.00 06/09
07/26/2010 11:13

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	11:13
02 Std. Gas	0.080	11:14
03 Room Air	0.000	11:14
04 Std. Gas	0.080	11:15
05 Room Air	0.000	11:15
06 Std. Gas	0.080	11:15
07 Room Air	0.000	11:16

Lot No = 659357
Cyl No = 26
Exp Date = 09/03/2011
County = 18 Oper No. = 049907

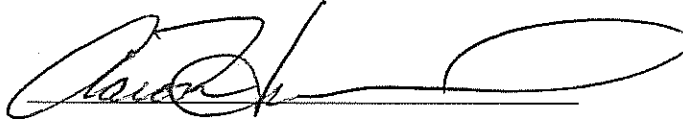

Operator Signature
AARON HUMMEL

Remarks: *ACA Test.*

Form 106-I8000

80-003057
P. 104 of 104
JTM