



INTOXILYZER® 8000 INSTALLATION AND REPAIR CHECKOUT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59281 (03-2014)

Serial Number <i>80-005950</i>	Instrument Location <i>FTOT BAT</i>
Reason for Install/Repair <input type="checkbox"/> Install After Receiving From Crime Laboratory <input checked="" type="checkbox"/> Install After Location Change <input type="checkbox"/> Other (Specify) _____	

Check When Done:

- 1. Surge Protector Installed/Properly Grounded.
- 2. Telephone Line Connected to Intoxilyzer® 8000.
- 3. Breath Tube Heated.
- 4. Enter Preliminary Data (i.e. Date, Time, DST (Y), and Location; Level 2, Function E).
- 5. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 6. Run Tests:
 - A. Print Test (Level 1, Function P).
 - B. ACA Test (Level 1, Function C).
 - C. RFI Test (CMS Mode or Level 1, Function B or C; Key Radio During Test).
- 7. Repair and/or Maintenance Performed (if Any): _____
- 8. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 9. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 10. Send the Following to the Crime Laboratory: Completed Intoxilyzer®8000 Installation and Repair Checkout (SFN59281, Form 104-G), Print Test, ACA Test, and RFI Test.

Field Inspector Signature <i>Jessie D. Moore</i>	Date <i>7-26-14</i> ✓
Reviewed By (Crime Laboratory Use Only) <i>Deb Kashur</i>	Date <i>15 Sept 14</i>

Intoxilyzer Test Record and Checklist
NDDAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005950
Location = FTOT 8164.13.00 06/09
07/26/2014 20:12

***** Printer Test *****

12 char/line
abcdefghijkl
ABCDEFGHIJKL

16 char per line
abcdefghijklmnop
ABCDEFGHIJKLMN

21 chars per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQRSTU

24 characters per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQRSTU

32 characters per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQRSTU

42 characters per line
abcdefghijklmnopqrstu
ABCDEFGHIJKLMNQRSTU

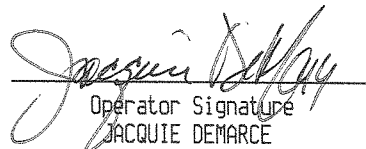
Current Instrument Setup
Data Entry Mode: Enabled
Start Test Sequence: DABACABA
Display Prelim Rslt? Yes
Display Third Digit? Yes
Inhib Printer(Y/N)? No
Display Volume? No
Disable On MemFull? Yes
of Print Copies? 1
Select Std (D/W/I)? Dry
Standard Value? 0.080
Standard Lot #: 33913080A4
Standard Cyl #: 46
Standard Expiration? 01/01/2016
Oper No? 100103

Flow Cal. Date: 06/20/2013
Slope 713
Intercept -723515

IR Calibration Date: 06/20/2013
3um 9um

0th Coef(*100): -37081 -23816
1st Coef(*100): 290549 133411
2nd Coef(*100): 552 1090
H2O adj(mg/l*10K): 683 502

***** Test End *****


Operator Signature
JACQUIE DEMARCE

Remarks:

Form 106-18000


Intoxilyzer Test Record and Checklist
NDDAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005950
Location = FTOT 8164.13.00 06/09
07/26/2014 20:16

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	20:17
02 Std. Gas	0.081	20:17
03 Room Air	0.000	20:18
04 Std. Gas	0.080	20:18
05 Room Air	0.000	20:19
06 Std. Gas	0.080	20:19
07 Room Air	0.000	20:19

Lot No = 33913080A4
Cyl No = 46
Exp Date = 01/01/2016
County = 03 Oper No. = 100103


Operator Signature
JACQUIE DEMARCE

Remarks:

Form 106-I8000

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

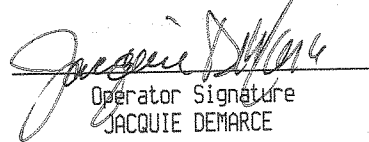
CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-005950
Location = FTOT 8164.13.00 06/09
07/26/2014 20:14

DRY CAL CHECK

Test	AC	Time
01 Room Air	RFI*	20:15
02 Room Air	0.000	20:16

*Invalid Test
Inhibited - RFI

Lot No = 33913080A4
Cyl No = 46
Exp Date = 01/01/2016
County = 03 Oper No. = 100103


Operator Signature
JACQUIE DEMARCE

Remarks: