




ETHANOL BREATH STANDARD CYLINDER REPORT


OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name:	Justin Cote				
Location:	Mohall North Dakota				
Intoxilyzer® Serial Number:	80-004198				
Gas Lot Number:	659358	Gas Cylinder Number:	27	Expiration Date:	09/03/11
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed				
Instrument Test Results (Report to 3 Digits; Example, 0.081%)					
Test 1: 0.077 %					
Test 2: 0.076 %					
Test 3: 0.077 %					
(ATTACH TEST RECORD)					

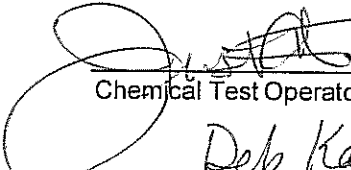

Chemical Test Operator Signature



Reviewed By

08/02/10
Date

03 Aug 2010
Date

80-004198
P. 92/98
JK

Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = MOHL 8164.13.00 06/09
08/02/2010 13:11

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	13:11
02 Std. Gas	0.077	13:12
03 Room Air	0.000	13:12
04 Std. Gas	0.076	13:13
05 Room Air	0.000	13:13
06 Std. Gas	0.077	13:14
07 Room Air	0.000	13:14


Lot No = 659358

Cyl No = 27

Exp Date = 09/03/2011

County = 38

Oper No. = 100913

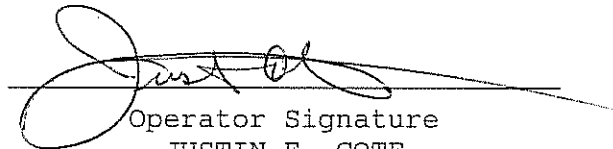
Operator Signature
JUSTIN E. COTE

Remarks:

Form 106-I8000

80-004198
P. 98 of 98
JEC