



# ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL  
CRIME LABORATORY DIVISION  
Toxicology Section/Breath Alcohol Program  
SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Chris Pulver</u>		
Location: <u>Mountrail 50</u>		
Intoxilyzer® Serial Number: <u>80-004943</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>34</u>	Expiration Date: <u>12-23-11</u>
<input type="checkbox"/> New Cylinder Installed	<input checked="" type="checkbox"/> Cylinder Not Changed	
Instrument Test Results (Report to 3 Digits; Example, 0.081%)		
Test 1: 0. <u>078</u> %		
Test 2: 0. <u>078</u> %		
Test 3: 0. <u>078</u> %		
(ATTACH TEST RECORD)		

Chris Pulver  
Chemical Test Operator Signature

8-8-10  
Date

Debi Kashner  
Reviewed By

10 Aug 2010  
Date

80-004943  
P. 49 of 50  
AK

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004943  
Location = STAN      8164.13.00 06/09  
08/08/2010      19:21

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	19:22
02 Std. Gas	0.078	19:22
03 Room Air	0.000	19:23
04 Std. Gas	0.078	19:23
05 Room Air	0.000	19:24
06 Std. Gas	0.078	19:24
07 Room Air	0.000	19:24


Lot No = 709352

Cyl No = 34

Exp Date = 12/23/2011

County = 31

Oper No. = 049912

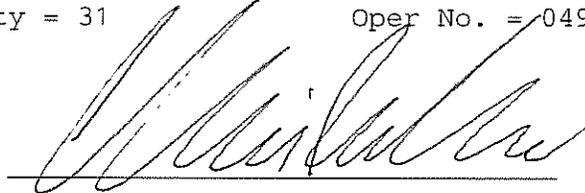

Operator Signature  
CHRISTOPHER PULVER

Remarks:

Form 106-I8000

80-004943  
P. 50 of 50  
KM