



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (5-2011)

Chemical Test Operator Name (Print) <i>Jonathan Lampi</i>		
Location <i>GFPD</i>	Intoxilyzer® Serial Number <i>80-009198</i>	
Gas Lot Number <i>23411080A1</i>	Gas Cylinder Number <i>02</i>	Gas Expiration Date <i>10-01-13</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 - A. *0.080* AC
 - B. *0.081* AC
 - C. *0.080* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Breath Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature <i>Jonathan Lampi</i>	Date <i>08-11-12</i>
Reviewed By (Crime Laboratory Use Only) <i>Deb Keshur</i>	Date <i>15 Aug 2012</i>

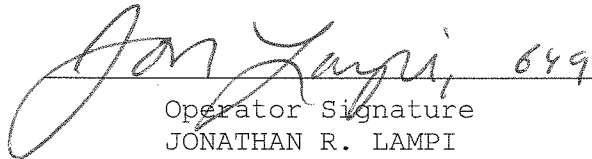
Intoxilyzer Test Record and Checklist
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004198
Location = GFPD 8164.13.00 06/09
08/11/2012 03:22

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	03:23
02 Std. Gas	0.080	03:23
03 Room Air	0.000	03:24
04 Std. Gas	0.081	03:24
05 Room Air	0.000	03:25
06 Std. Gas	0.080	03:25
07 Room Air	0.000	03:25

Lot No = 23411080A1
Cyl No = 62
Exp Date = 10/01/2013
County = 18 Oper No. = 039947


Operator Signature
JONATHAN R. LAMPI

Remarks:

Form 106-I8000

ACA for cylinder change