



ETHANOL BREATH STANDARD CYLINDER REPORT

OFFICE OF ATTORNEY GENERAL
CRIME LABORATORY DIVISION
Toxicology Section/Breath Alcohol Program
SFN 59282 (5-2011)

Chemical Test Operator Name (Print) <i>Janie M Huschka</i>		
Location <i>Williams Co LEC</i>		Intoxilyzer® Serial Number <i>80-004950</i>
Gas Lot Number <i>16512080A2</i>	Gas Cylinder Number <i>61</i>	Gas Expiration Date <i>03/01/2014</i>

Check When Done:

- 1. Scan/Enter Gas Cylinder Information (Level 1, Function S).
- 2. Perform an ACA Test (Level 1, Function C).
Write in the ACA Test Results (Reported to 3 Digits, Ex. 0.081).
 - A. *0.079* AC
 - B. *0.080* AC
 - C. *0.080* AC
- 3. Complete the Top Portion of the Intoxilyzer® Record (SFN50496, Form 120-G) and Place it by the Intoxilyzer® for Use.
- 4. File Previous Intoxilyzer® Record (SFN50496, Form 120-G) at the Intoxilyzer® Location at the Agency.
- 5. Send the Following to the Crime Laboratory:
 - A. Ethanol Breath Standard Cylinder Report (SFN59282, Form 105-G).
 - B. ACA Test Record.

Chemical Test Operator Signature <i>Janie M Huschka</i>	Date <i>24 Aug 13</i>
Reviewed By (Crime Laboratory Use Only) <i>Deb Kashur</i>	Date <i>03 Sept '13</i>

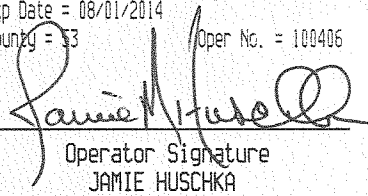
Intoxilyzer Test Record and Checklist
NDOCAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer Alcohol Analyzer
North Dakota Model 8000 SN 80-004950
Location = WILL 8164.13.00 06/09
08/24/2013 18:37

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	18:38
02 Std. Gas	0.079	18:38
03 Room Air	0.000	18:39
04 Std. Gas	0.080	18:39
05 Room Air	0.000	18:40
06 Std. Gas	0.080	18:40
07 Room Air	0.000	18:41

Lot No = 16512080A2
Cyl No = 61
Exp Date = 08/01/2014
County = 53 Oper No. = 100406


Operator Signature
JAMIE HUSCHKA

Remarks:

Form 106-18000