



**ETHANOL BREATH STANDARD CYLINDER REPORT**  
 OFFICE OF ATTORNEY GENERAL  
 CRIME LABORATORY DIVISION  
 Toxicology Section/Breath Alcohol Program  
 SFN 59282 (1-2010)

Only Chemical Test Operators may change the Ethanol Breath Standard and complete this form.

Chemical Test Operator Name: <u>Duane L. MARMON</u>		
Location: <u>STAN</u>		
Intoxilyzer® Serial Number: <u>80-004943</u>		
Gas Lot Number: <u>709352</u>	Gas Cylinder Number: <u>34</u>	Expiration Date: <u>12/23/11</u>
<input type="checkbox"/> New Cylinder Installed <input checked="" type="checkbox"/> Cylinder Not Changed		
Instrument Test Results (Report to 3 Digits; Example, 0.081%) Test 1: <u>0.078</u> % Test 2: <u>0.079</u> % Test 3: <u>0.078</u> %		
(ATTACH TEST RECORD)		

Chemical Test Operator Signature

09/04/10  
 Date

Deb Kashner  
 Reviewed By

09 Sept 2010  
 Date

80-004943  
 p. 51 of 52  
 KM

Intoxilyzer Test Record and Checklist  
NDOAG Crime Lab. Div., Bismarck, ND 58501

CMI, Inc. Intoxilyzer      Alcohol Analyzer  
North Dakota Model 8000      SN 80-004943  
Location = STAN      8164.13.00 06/09  
09/04/2010      19:28

DRY CAL CHECK

Test	AC	Time
01 Room Air	0.000	19:29
02 Std. Gas	0.078	19:29
03 Room Air	0.000	19:29
04 Std. Gas	0.079	19:30
05 Room Air	0.000	19:30
06 Std. Gas	0.078	19:31
07 Room Air	0.000	19:31


Lot No = 709352

Cyl No = 34

Exp Date = 12/23/2011

County = 31

Oper No. = 100019

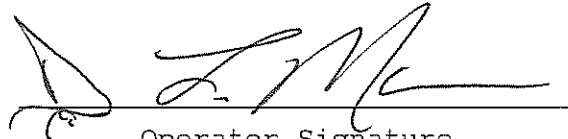

Operator Signature  
DUANE L. MARMON

Remarks:

Form 106-I8000

80-004943  
P. 52 of 52  
AM